

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111424\
 Data File : P0107993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2024 23:53
 Operator : YP/AJ
 Sample : P4835-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 345-2-WATER

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :Ankita Jodhani 11/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 01:48:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 12 01:21:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.381	3.657	65105571	26817307	7.253m	7.985
2) SA Decachlor...	10.088	8.636	26561755	22904545	8.960	7.250

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111424\
Data File : PO107993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2024 23:53
Operator : YP/AJ
Sample : P4835-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
345-2-WATER


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :Ankita Jodhani 11/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 01:48:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111124.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 12 01:21:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

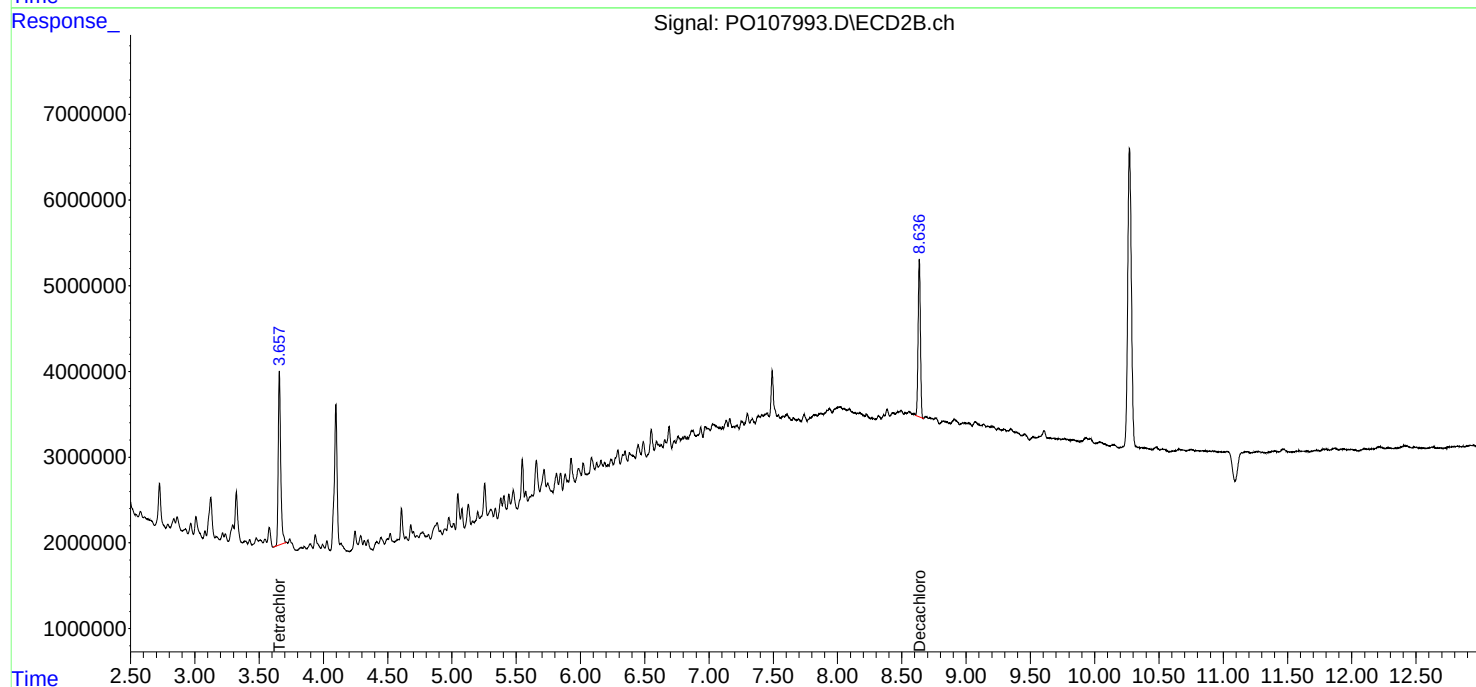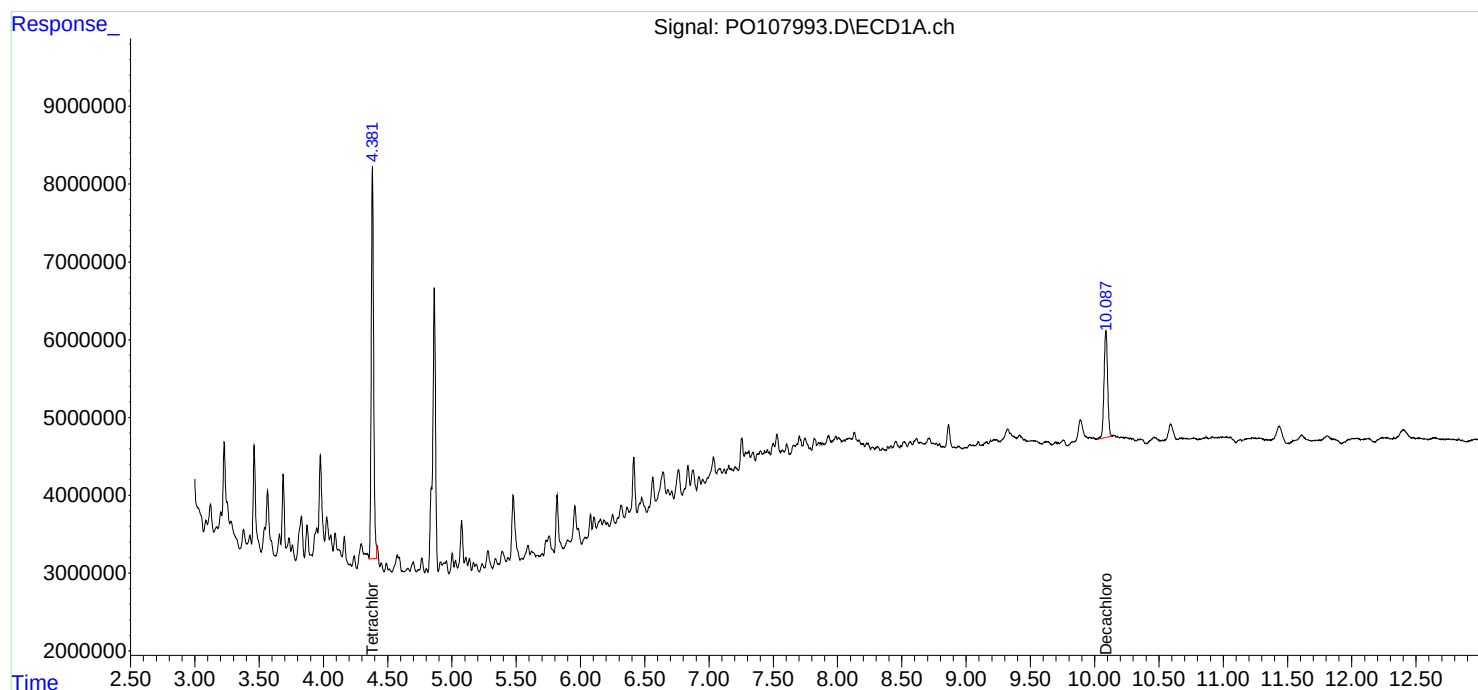

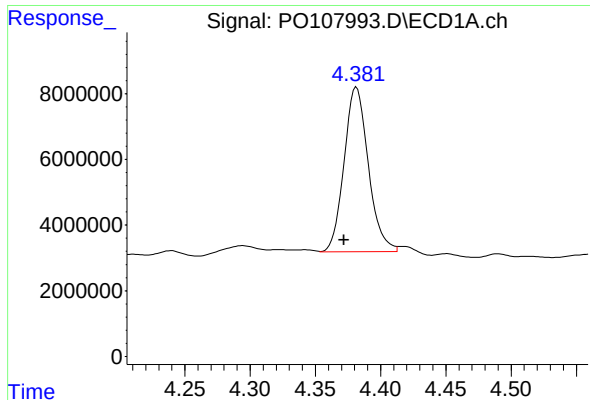


#1 Tetrachloro-m-xylene

R.T.: 4.381 min
Delta R.T.: 0.009 min
Response: 65105571
Conc: 7.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
345-2-WATER


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :Ankita Jodhani 11/15/2024

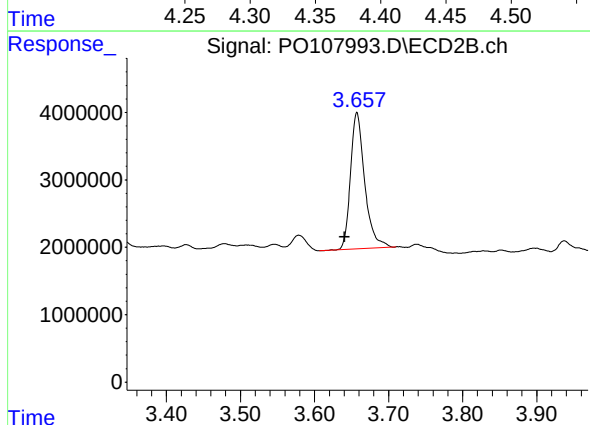


#1 Tetrachloro-m-xylene

R.T.: 3.657 min
Delta R.T.: 0.016 min
Response: 26817307
Conc: 7.98 ng/ml

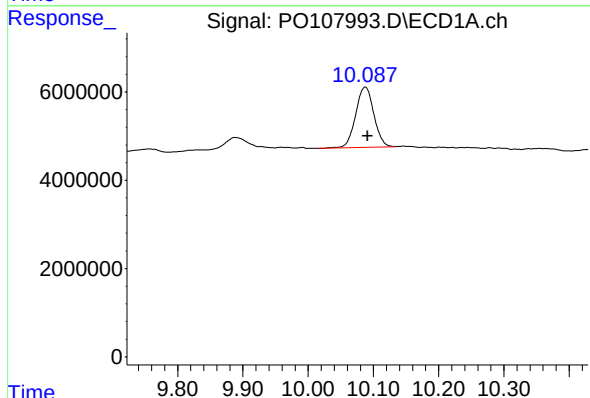

#2 Decachlorobiphenyl

R.T.: 10.088 min
Delta R.T.: -0.004 min
Response: 26561755
Conc: 8.96 ng/ml

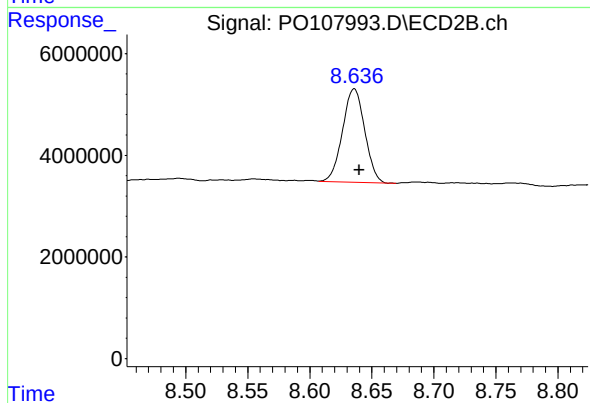

#2 Decachlorobiphenyl

R.T.: 8.636 min
Delta R.T.: -0.004 min
Response: 22904545
Conc: 7.25 ng/ml