

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111519\
 Data File : P0063752.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Nov 2019 17:42
 Operator : SM/AJ
 Sample : K5860-05
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20983-32007

Manual Integrations
 APPROVED

Ankita
 11/18/2019 2:54:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 03:36:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.317	3.573	1092979	719107	35.747m	32.376
2)	SA Decachlor...	9.939	8.539	778970	540439	19.170	18.479

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111519\
Data File : PO063752.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Nov 2019 17:42
Operator : SM/AJ
Sample : K5860-05
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20983-32007


Manual Integrations
APPROVED

Ankita
11/18/2019 2:54:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 03:36:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

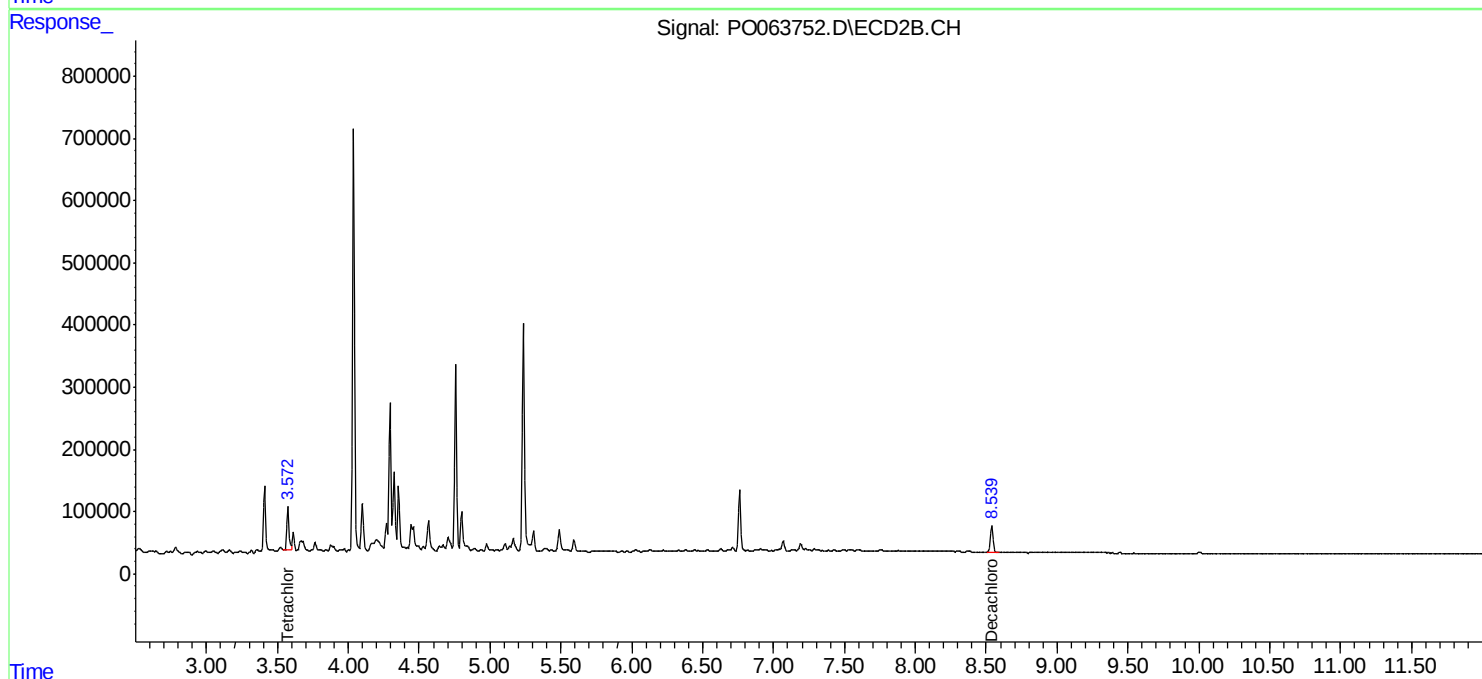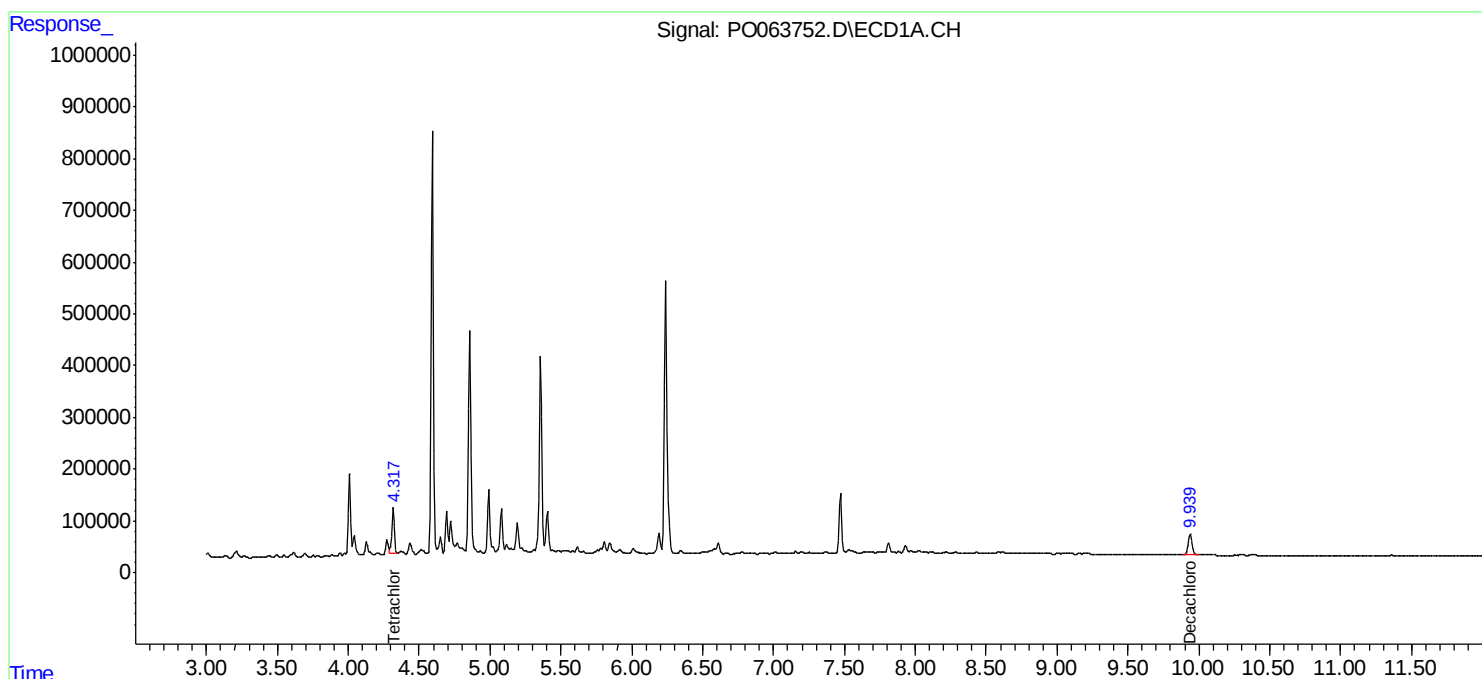

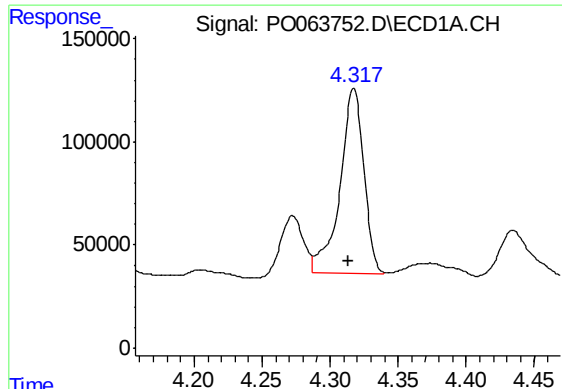


#1 Tetrachloro-m-xylene

R.T.: 4.317 min
Delta R.T.: 0.003 min
Response: 1092979
Conc: 35.75 ng/ml m

Instrument :
ECD_O
ClientSampleId :
20983-32007


Manual Integrations
APPROVED

Ankita
11/18/2019 2:54:18 PM

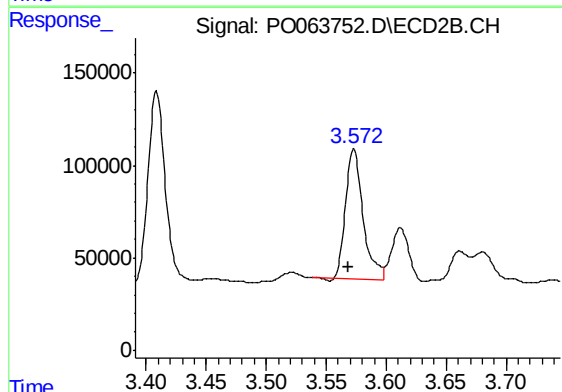


#1 Tetrachloro-m-xylene

R.T.: 3.573 min
Delta R.T.: 0.004 min
Response: 719107
Conc: 32.38 ng/ml

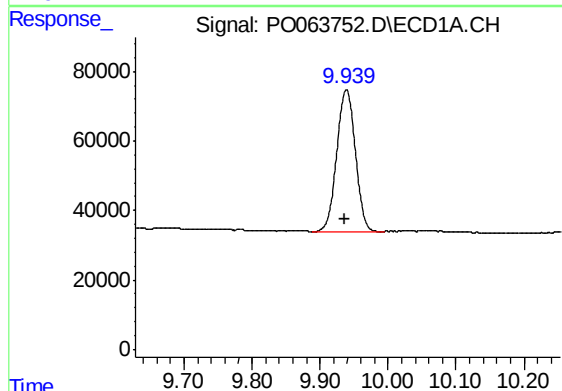

#2 Decachlorobiphenyl

R.T.: 9.939 min
Delta R.T.: 0.003 min
Response: 778970
Conc: 19.17 ng/ml

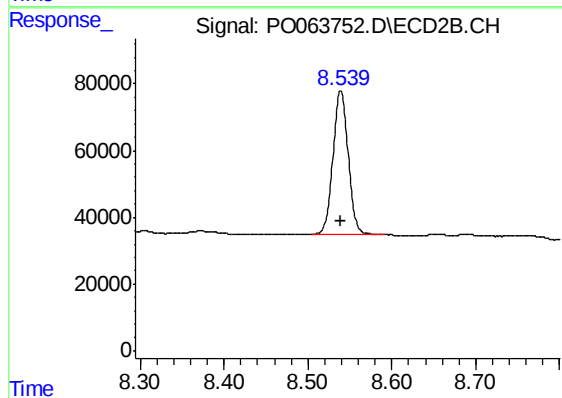

#2 Decachlorobiphenyl

R.T.: 8.539 min
Delta R.T.: 0.000 min
Response: 540439
Conc: 18.48 ng/ml