

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111519\
 Data File : P0063774.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Nov 2019 00:20
 Operator : SM/AJ
 Sample : K5860-09
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20777

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 03:43:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.316	3.570	589585	438521	19.283	19.743
2) SA Decachlor...	9.939	8.538	476263	431408	11.721	14.751 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111519\
Data File : P0063774.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Nov 2019 00:20
Operator : SM/AJ
Sample : K5860-09
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20777

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 03:43:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

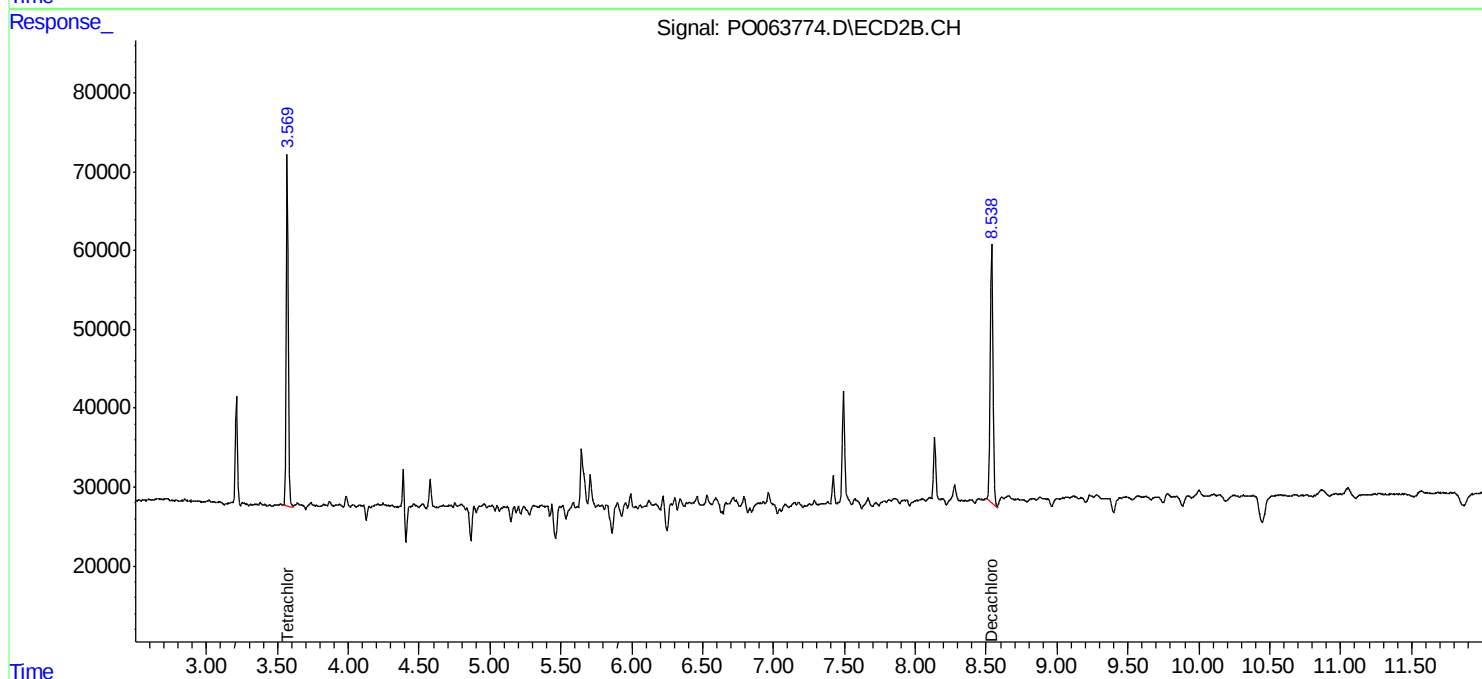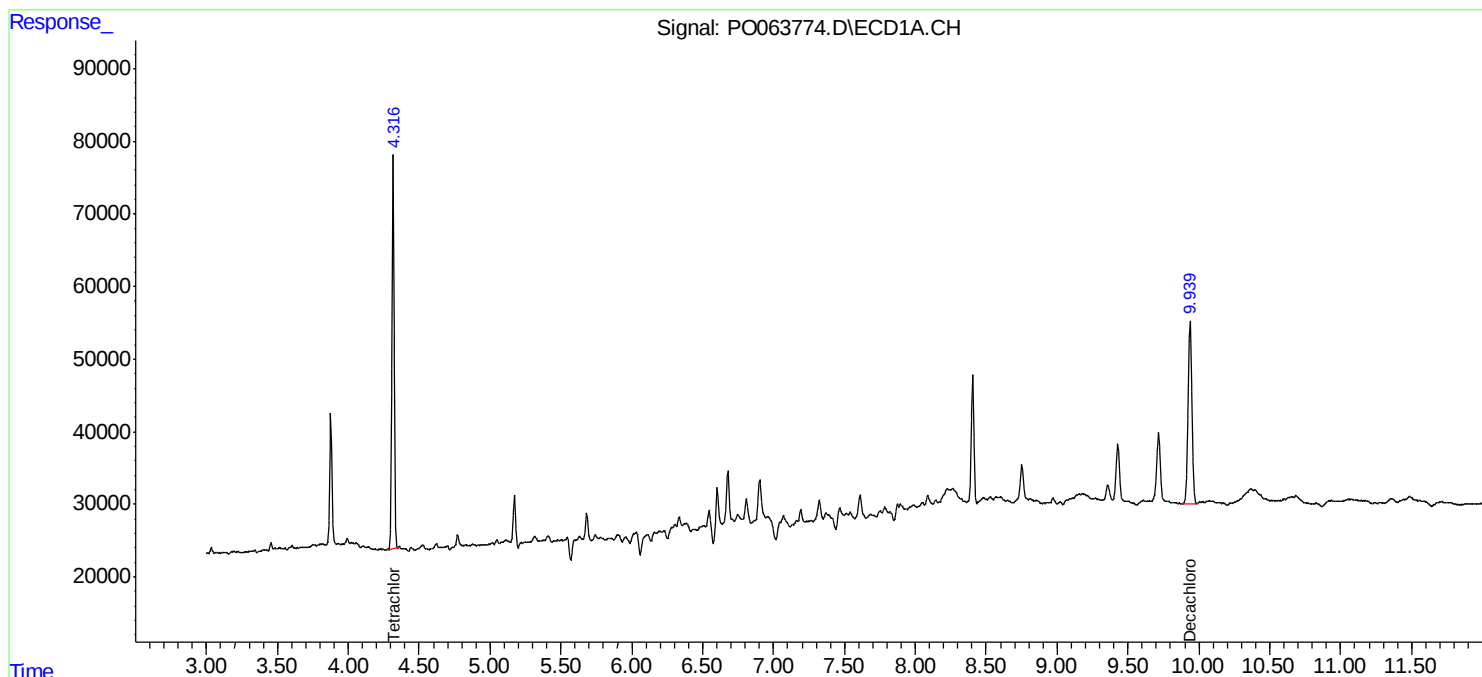


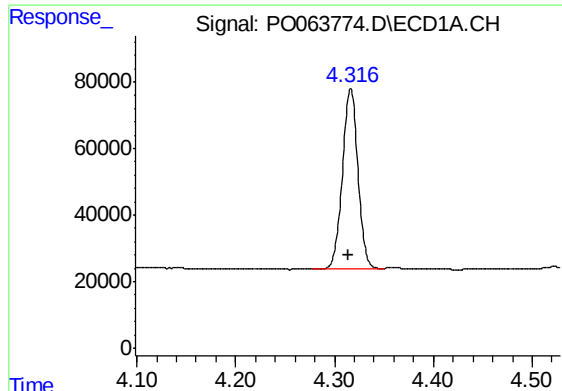

#1 Tetrachloro-m-xylene


R.T.: 4.316 min
Delta R.T.: 0.002 min
Response: 589585
Conc: 19.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
20777

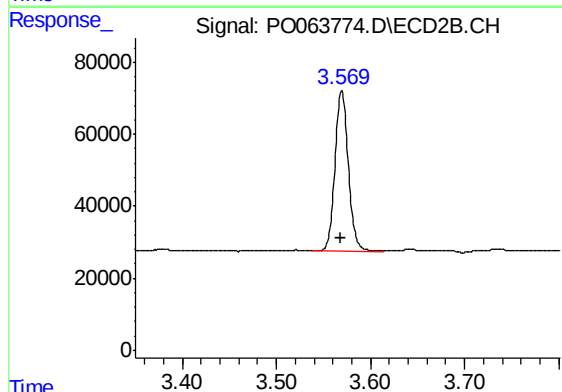


#1 Tetrachloro-m-xylene

R.T.: 3.570 min
Delta R.T.: 0.000 min
Response: 438521
Conc: 19.74 ng/ml

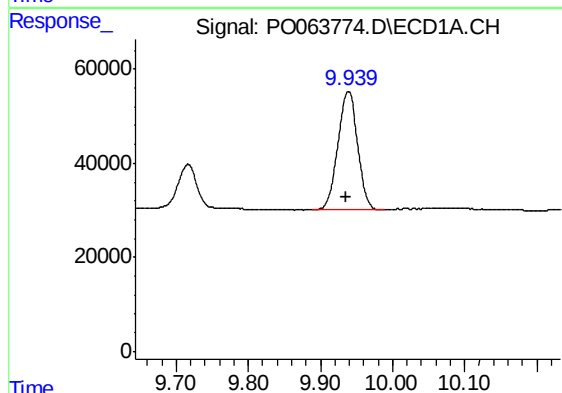

#2 Decachlorobiphenyl

R.T.: 9.939 min
Delta R.T.: 0.003 min
Response: 476263
Conc: 11.72 ng/ml

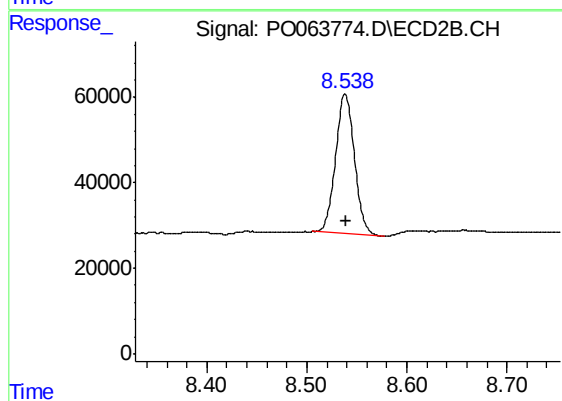

#2 Decachlorobiphenyl

R.T.: 8.538 min
Delta R.T.: -0.001 min
Response: 431408
Conc: 14.75 ng/ml