

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111521\
 Data File : PO082919.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Nov 2021 21:45
 Operator : AJ\MA
 Sample : M4687-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VWE-B35-111221-0-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 01:26:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.959	3.958	1619830	559249	18.166	17.235
2) SA Decachlor...	11.058	9.269	1063396	457012	18.361	16.119

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111521\
Data File : P0082919.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Nov 2021 21:45
Operator : AJ\MA
Sample : M4687-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
VWE-B35-111221-0-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 01:26:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

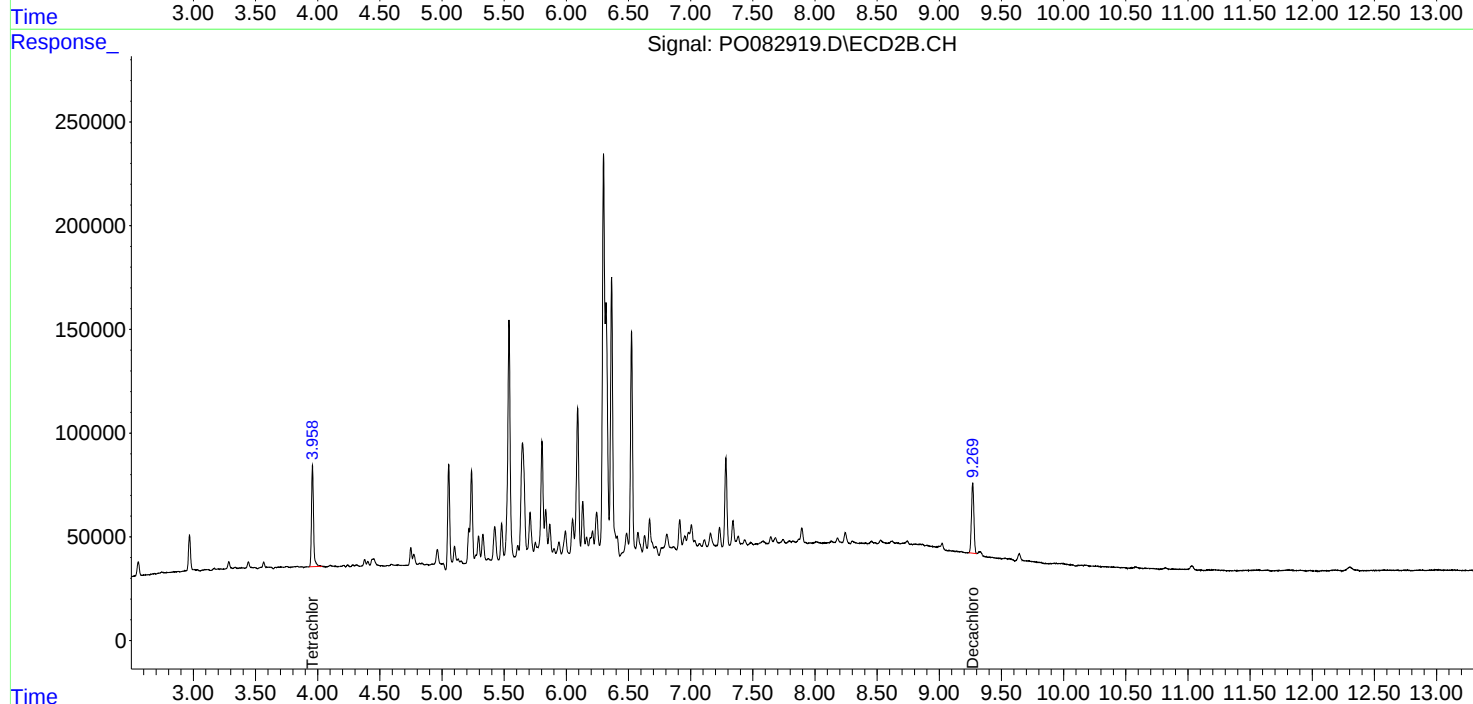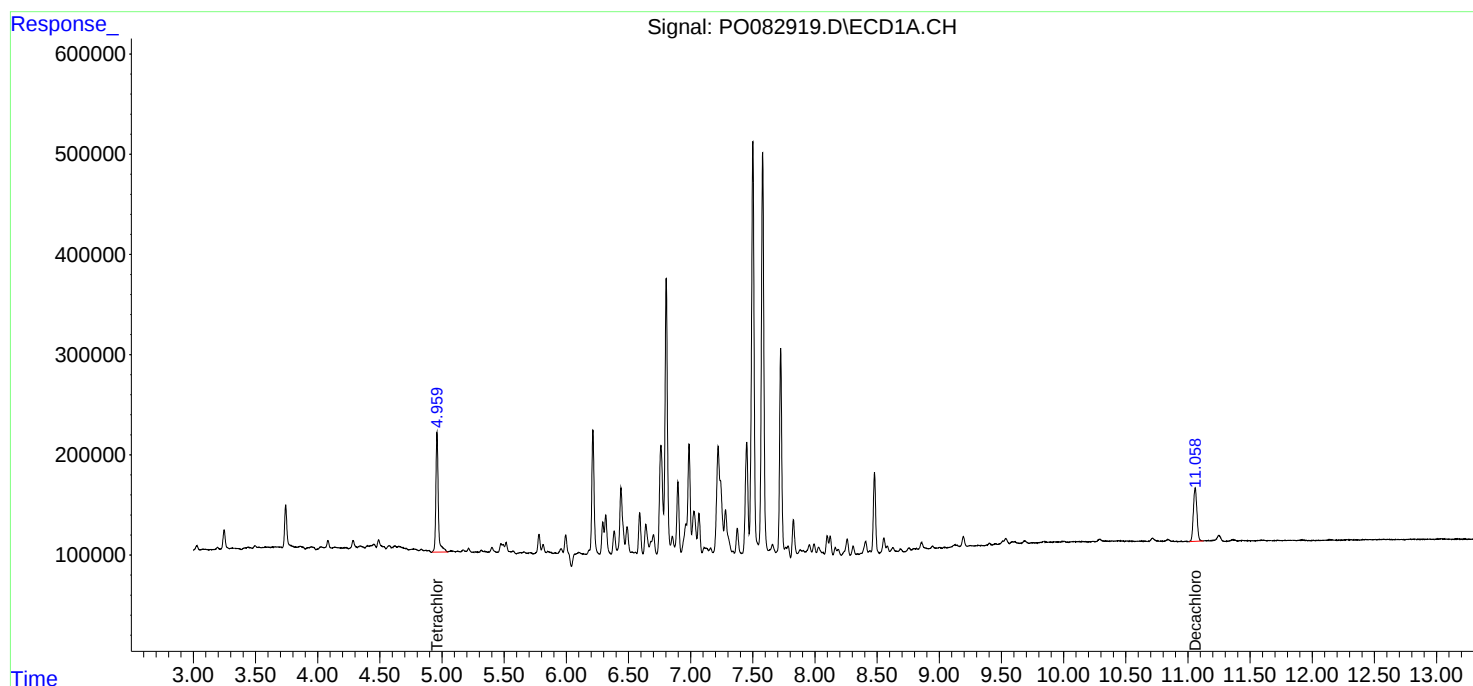


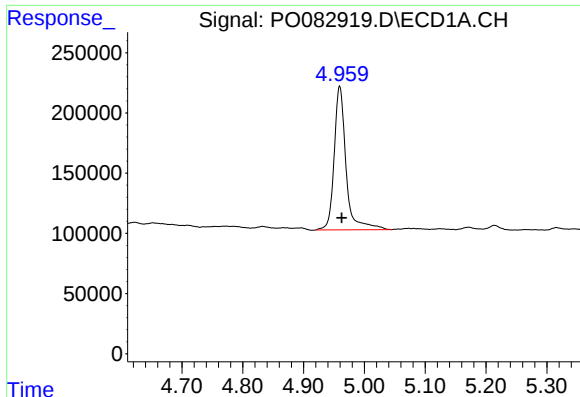

#1 Tetrachloro-m-xylene


R.T.: 4.959 min
Delta R.T.: -0.004 min
Response: 1619830
Conc: 18.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
VWE-B35-111221-0-10

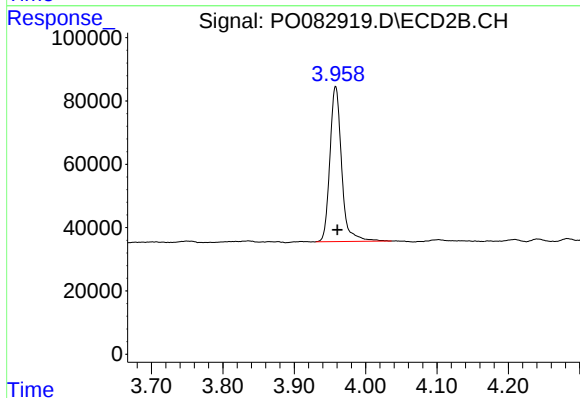


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: -0.003 min
Response: 559249
Conc: 17.23 ng/ml

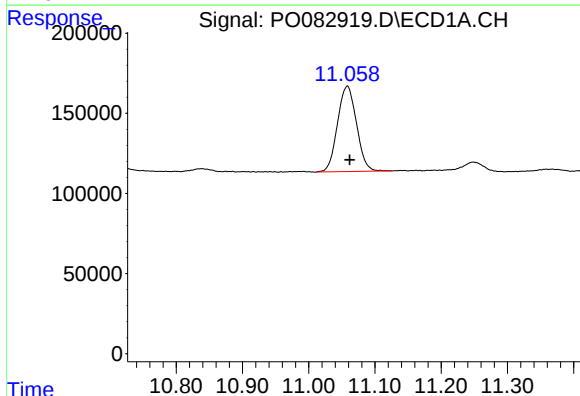

#2 Decachlorobiphenyl

R.T.: 11.058 min
Delta R.T.: -0.004 min
Response: 1063396
Conc: 18.36 ng/ml

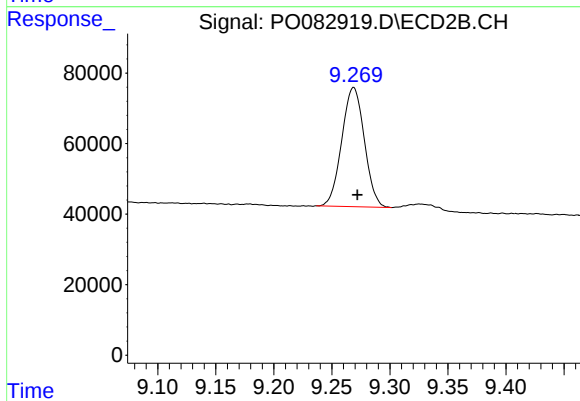

#2 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: -0.003 min
Response: 457012
Conc: 16.12 ng/ml