

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111522\
 Data File : PO090627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 05:05
 Operator : YP/AJ
 Sample : N5618-07 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC254708LOZ-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/16/2022
 Supervised By :Ankita Jodhani 11/16/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 06:14:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.301	3.479	5337665	1774045	1.661	1.669
2) SA Decachlor...	10.056	8.488	6997312	1615313	2.855	1.568m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111522\
Data File : PO090627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 05:05
Operator : YP/AJ
Sample : N5618-07 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC254708LOZ-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/16/2022
Supervised By :Ankita Jodhani 11/16/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 06:14:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

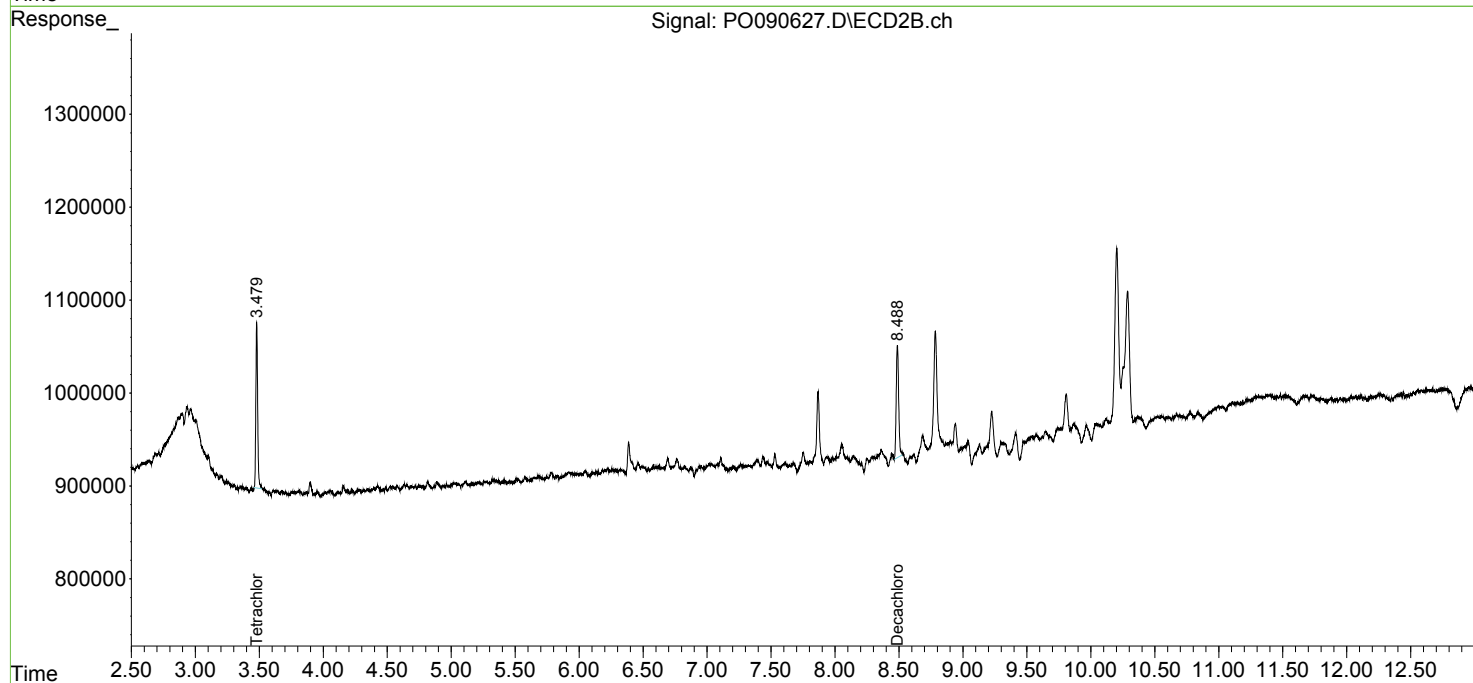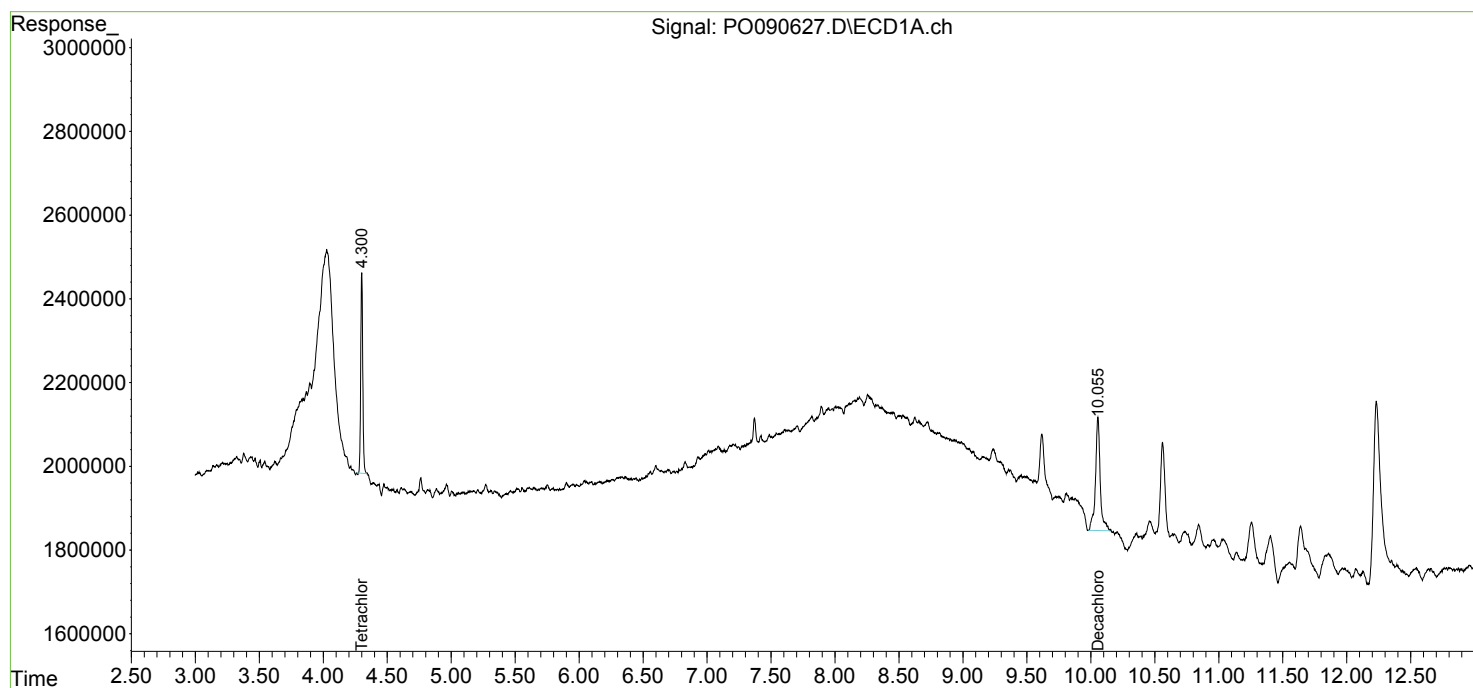

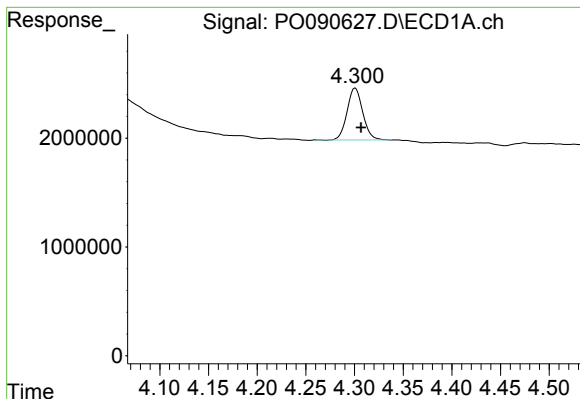


#1 Tetrachloro-m-xylene

R.T.: 4.301 min
Delta R.T.: -0.006 min
Response: 5337665
Conc: 1.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC254708LOZ-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/16/2022
Supervised By :Ankita Jodhani 11/16/2022

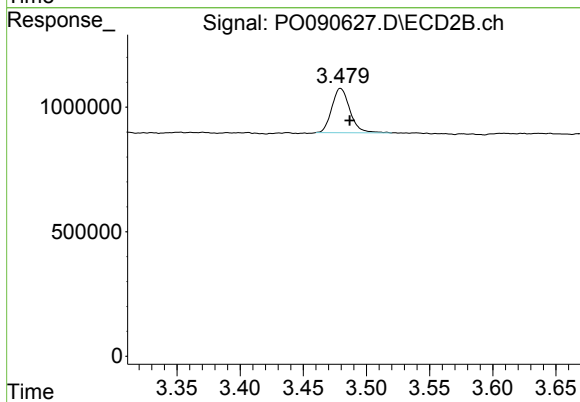


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: -0.007 min
Response: 1774045
Conc: 1.67 ng/ml

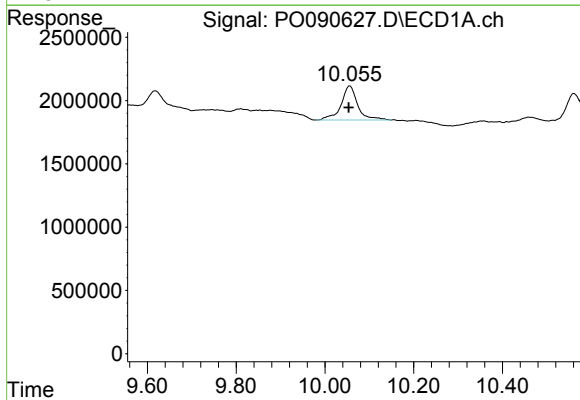

#2 Decachlorobiphenyl

R.T.: 10.056 min
Delta R.T.: 0.002 min
Response: 6997312
Conc: 2.86 ng/ml

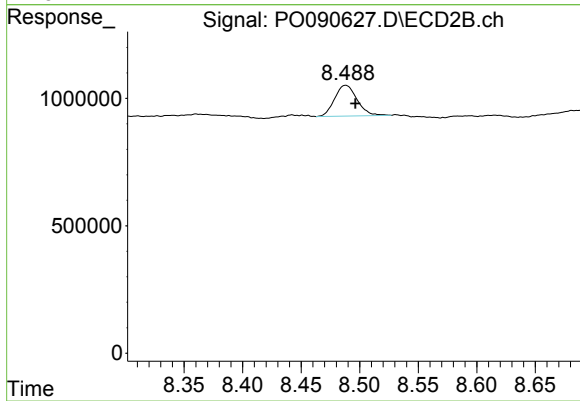

#2 Decachlorobiphenyl

R.T.: 8.488 min
Delta R.T.: -0.009 min
Response: 1615313
Conc: 1.57 ng/ml m