

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111523\
 Data File : PO099820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2023 01:01
 Operator : YP/AJ
 Sample : 05408-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 710-NEW-YORK-AVE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/16/2023
 Supervised By :Ankita Jodhani 11/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 02:05:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 14 04:21:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.490	3.716	32232671	24804580	18.848	20.999
2) SA Decachlor...	10.370	8.815	17851193	18710711	19.119	19.063m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111523\
Data File : PO099820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2023 01:01
Operator : YP/AJ
Sample : 05408-01
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
710-NEW-YORK-AVE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/16/2023
Supervised By :Ankita Jodhani 11/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 02:05:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 14 04:21:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

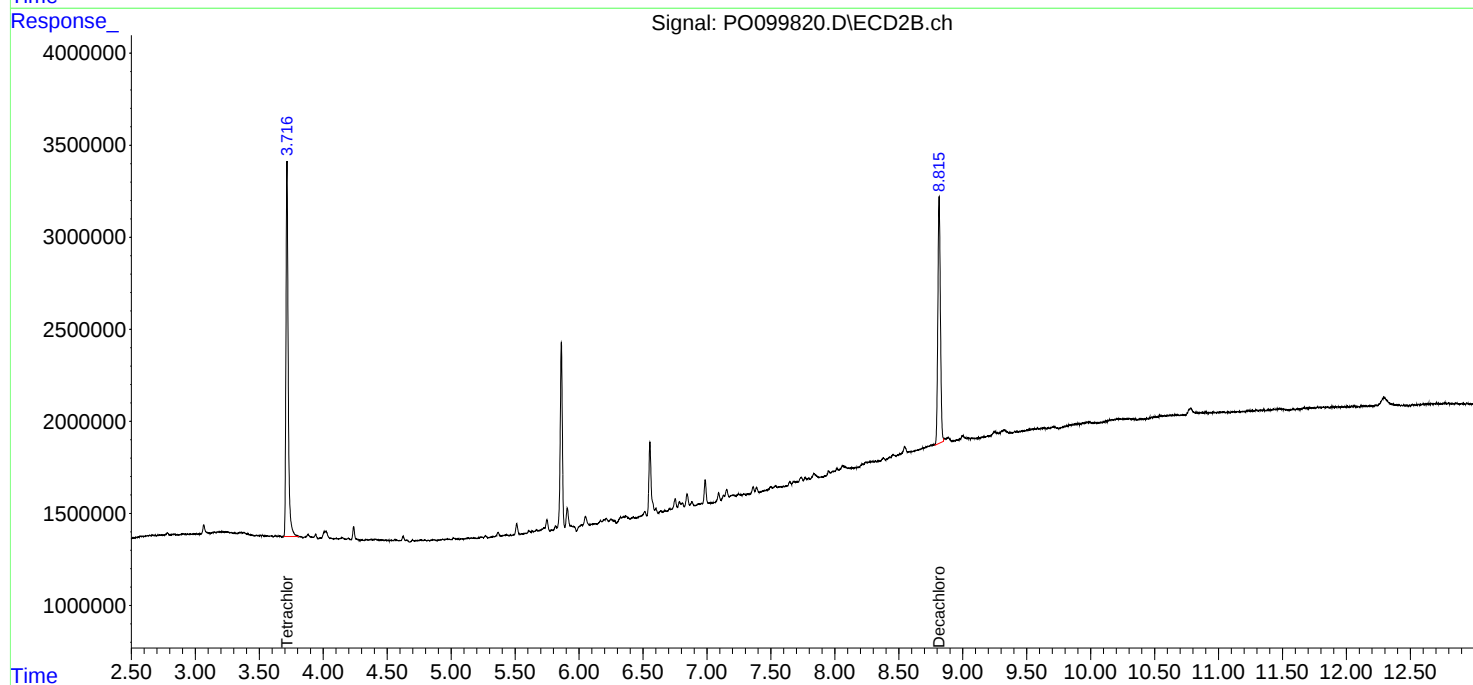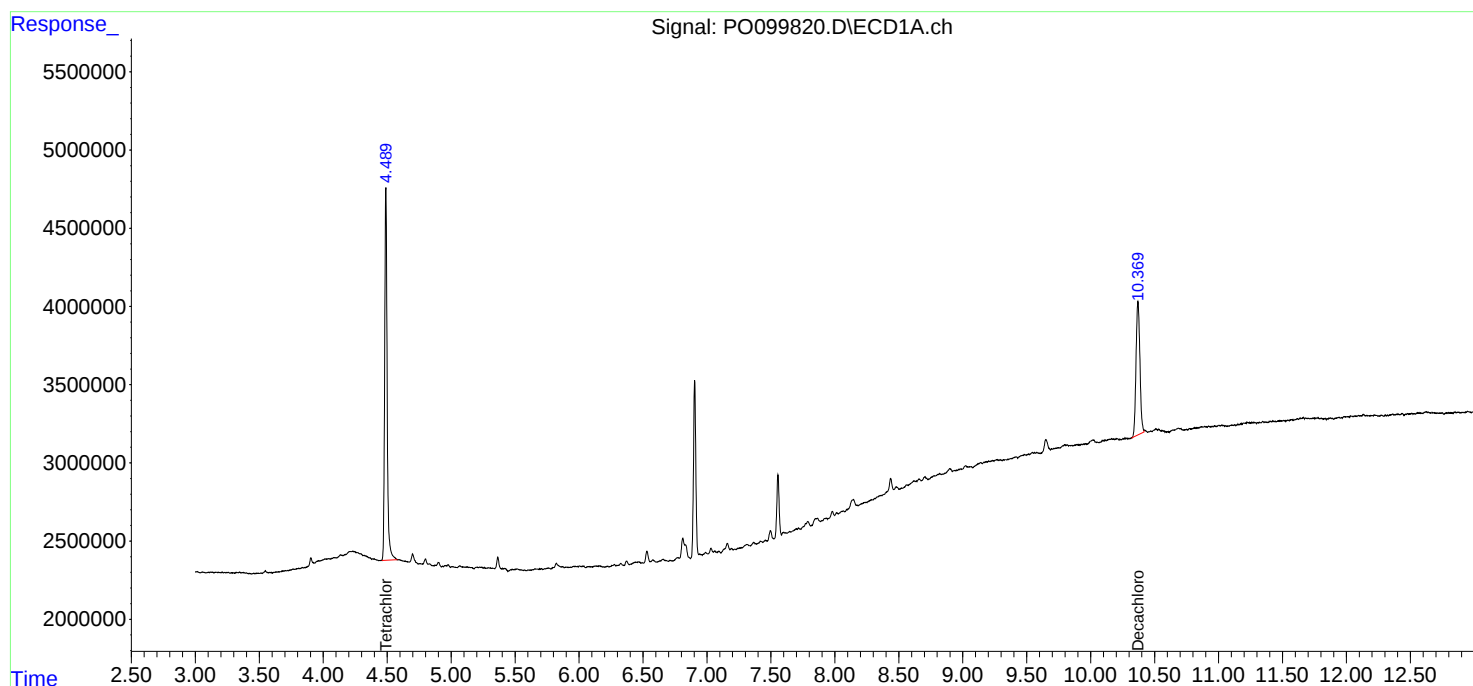

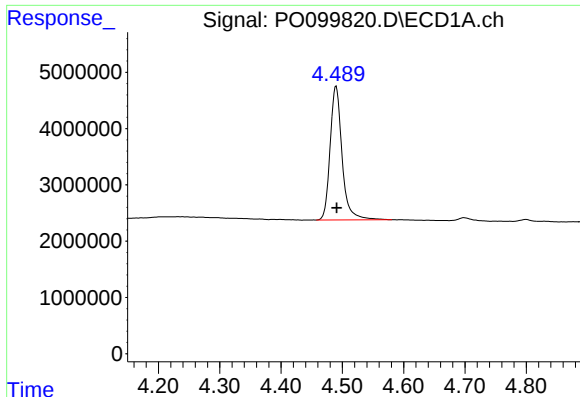


#1 Tetrachloro-m-xylene

R.T.: 4.490 min
Delta R.T.: -0.001 min
Response: 32232671
Conc: 18.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
710-NEW-YORK-AVE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/16/2023
Supervised By :Ankita Jodhani 11/16/2023

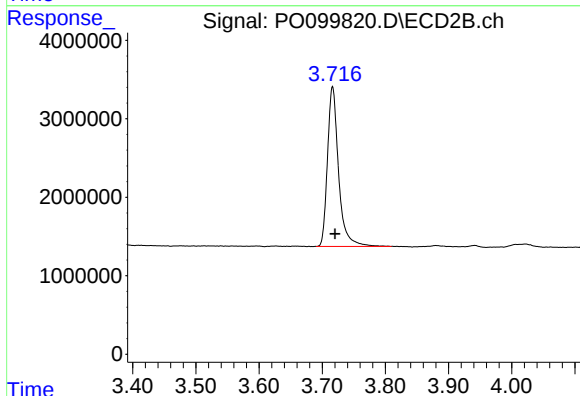


#1 Tetrachloro-m-xylene

R.T.: 3.716 min
Delta R.T.: -0.004 min
Response: 24804580
Conc: 21.00 ng/ml

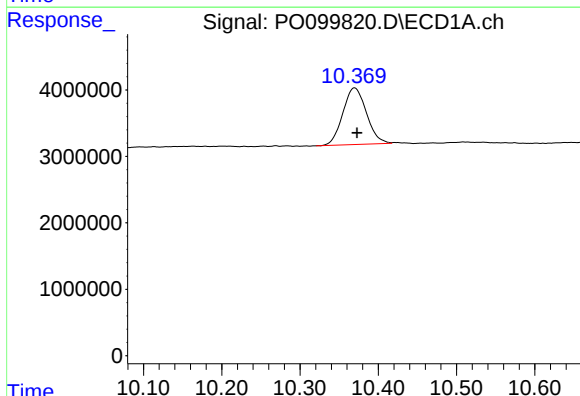

#2 Decachlorobiphenyl

R.T.: 10.370 min
Delta R.T.: -0.003 min
Response: 17851193
Conc: 19.12 ng/ml

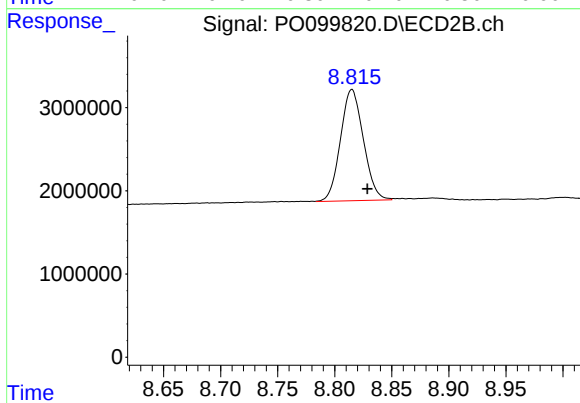

#2 Decachlorobiphenyl

R.T.: 8.815 min
Delta R.T.: -0.014 min
Response: 18710711
Conc: 19.06 ng/ml m