

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111523\
 Data File : P0099843.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2023 07:58
 Operator : YP/AJ
 Sample : 05414-15
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 15-A-15-B-15-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/16/2023
 Supervised By :Ankita Jodhani 11/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 08:05:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 14 04:21:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.490	3.716	38531436	28911561	22.532	24.476
2) SA Decachlor...	10.369	8.816	24485407	25166897	26.225	25.640m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111523\
Data File : PO099843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2023 07:58
Operator : YP/AJ
Sample : 05414-15
Misc :
ALS Vial : 59 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
15-A-15-B-15-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/16/2023
Supervised By :Ankita Jodhani 11/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 08:05:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 14 04:21:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

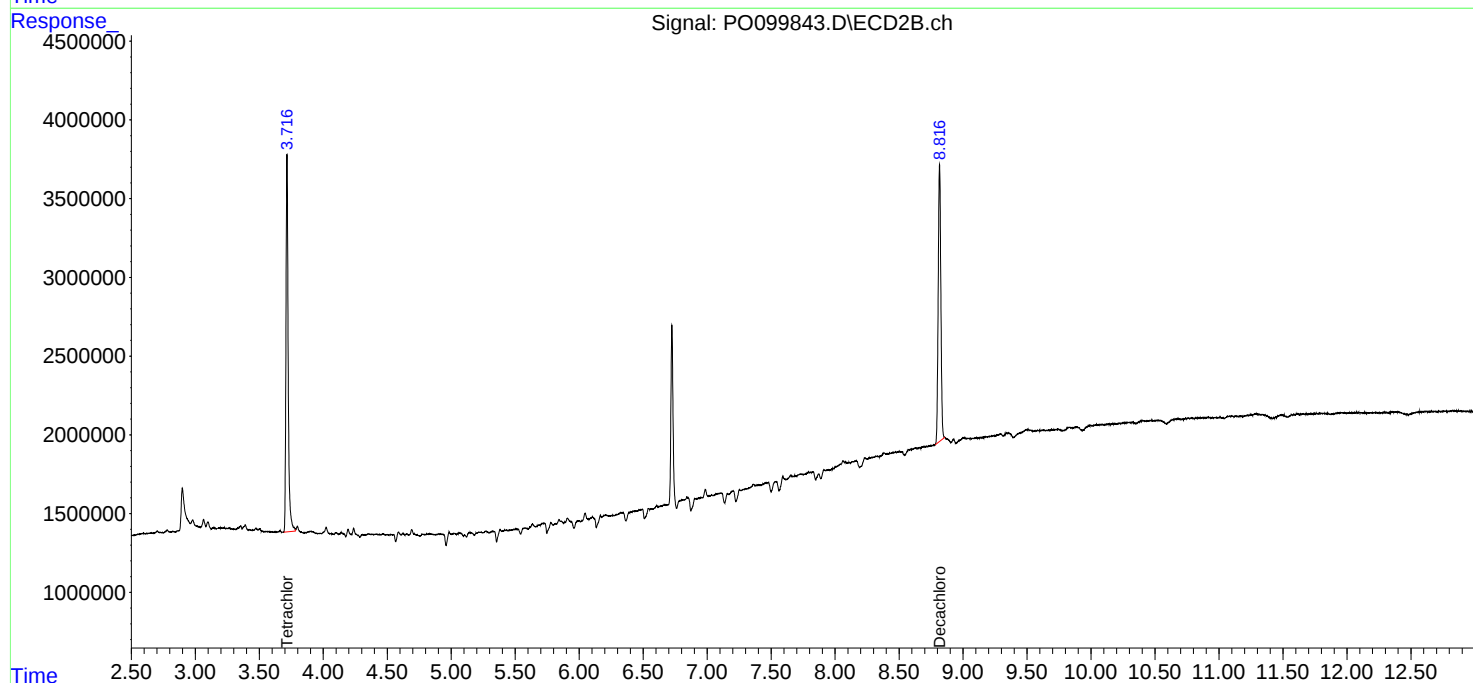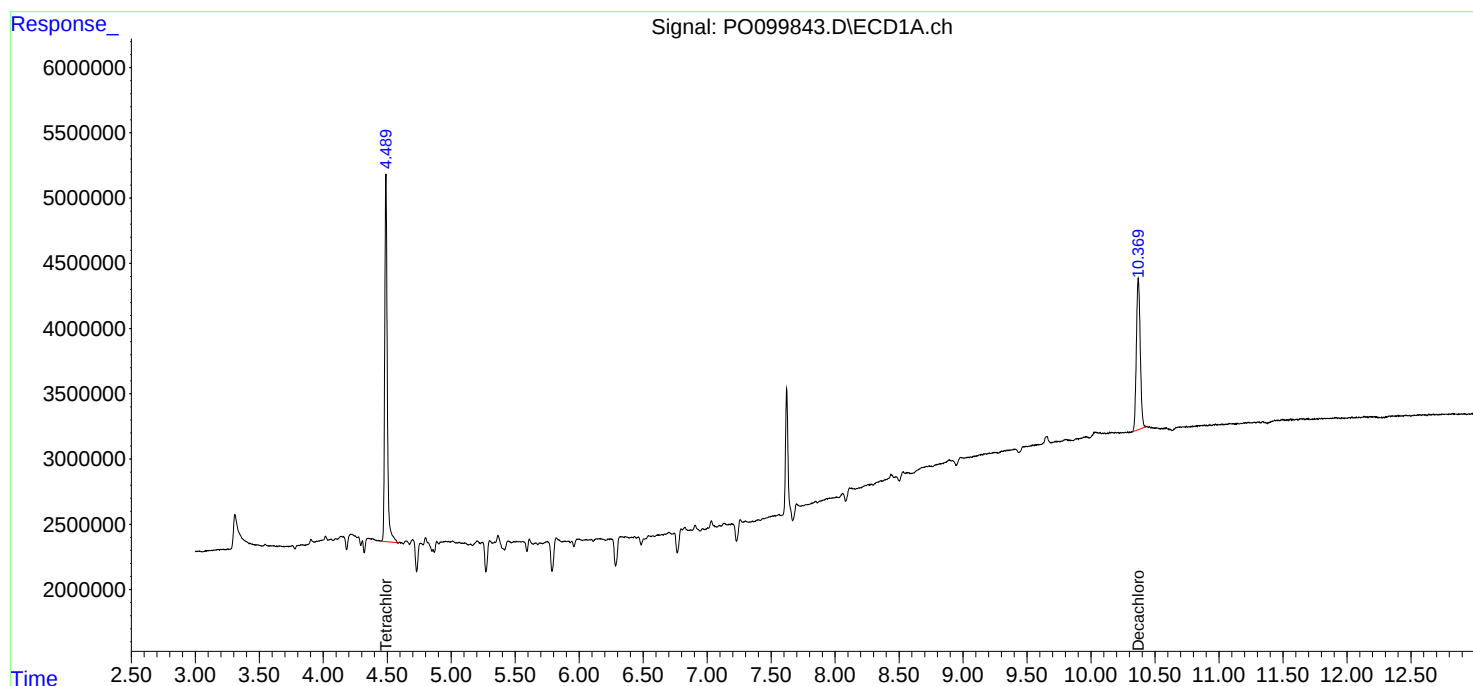

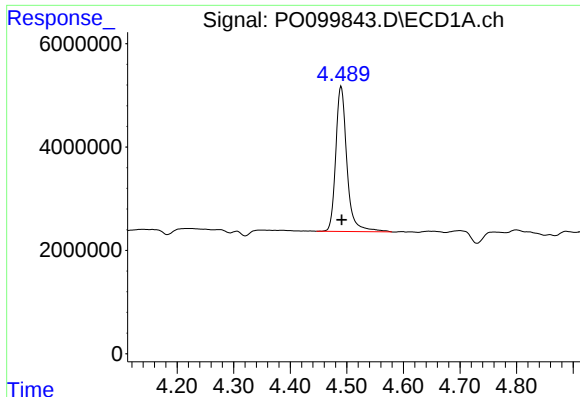


#1 Tetrachloro-m-xylene

R.T.: 4.490 min
Delta R.T.: -0.001 min
Response: 38531436
Conc: 22.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
15-A-15-B-15-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/16/2023
Supervised By :Ankita Jodhani 11/16/2023

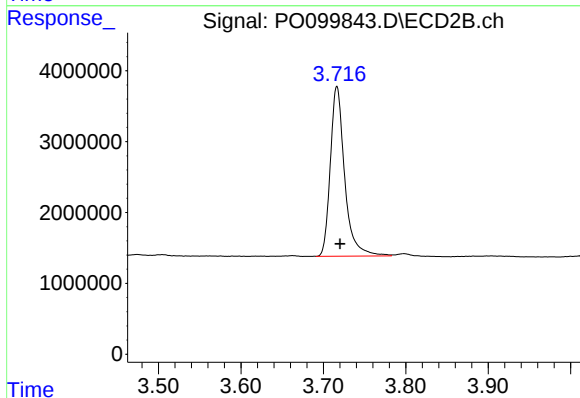


#1 Tetrachloro-m-xylene

R.T.: 3.716 min
Delta R.T.: -0.004 min
Response: 28911561
Conc: 24.48 ng/ml

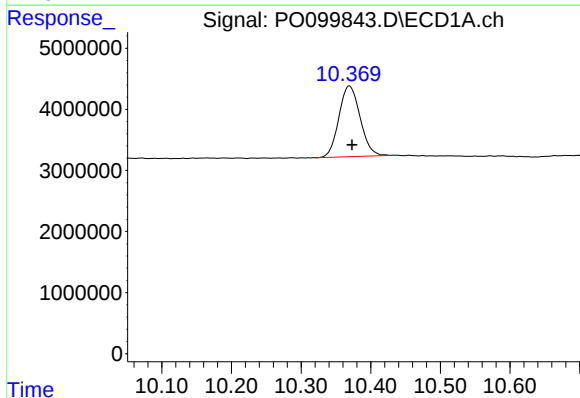

#2 Decachlorobiphenyl

R.T.: 10.369 min
Delta R.T.: -0.004 min
Response: 24485407
Conc: 26.22 ng/ml

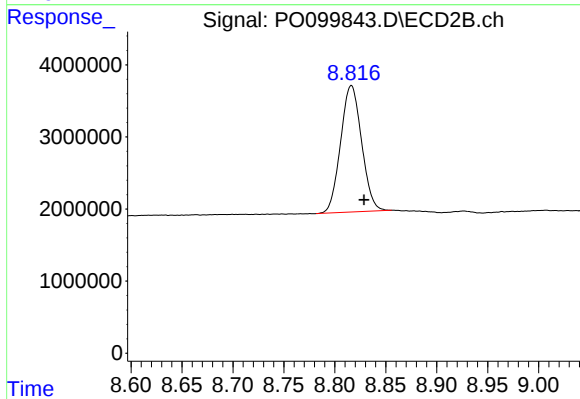

#2 Decachlorobiphenyl

R.T.: 8.816 min
Delta R.T.: -0.013 min
Response: 25166897
Conc: 25.64 ng/ml m