

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111618\
 Data File : P0051595.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Nov 2018 10:50
 Operator : SM/SJ
 Sample : J5939-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OILY-WATER

Manual Integrations
 APPROVED

Sohil
 11/19/2018 4:40:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 13:41:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 15 08:04:19 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.318	3.304	28389063	10132591	8.889	9.202
2) SA Decachlor...	9.969	8.059	8976422	4571686	4.677m	5.515m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111618\
Data File : PO051595.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Nov 2018 10:50
Operator : SM/SJ
Sample : J5939-01
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OILY-WATER


Manual Integrations
APPROVED

Sohil
11/19/2018 4:40:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 13:41:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111318.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 15 08:04:19 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

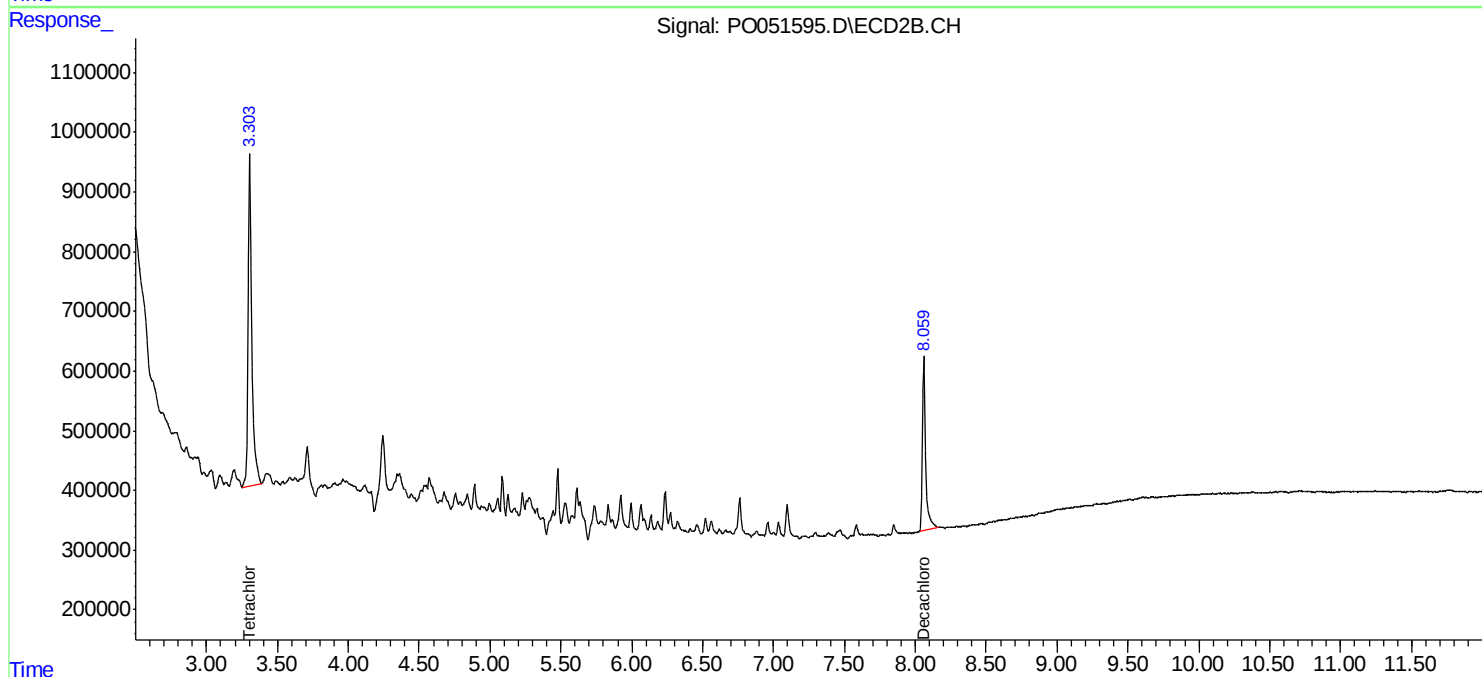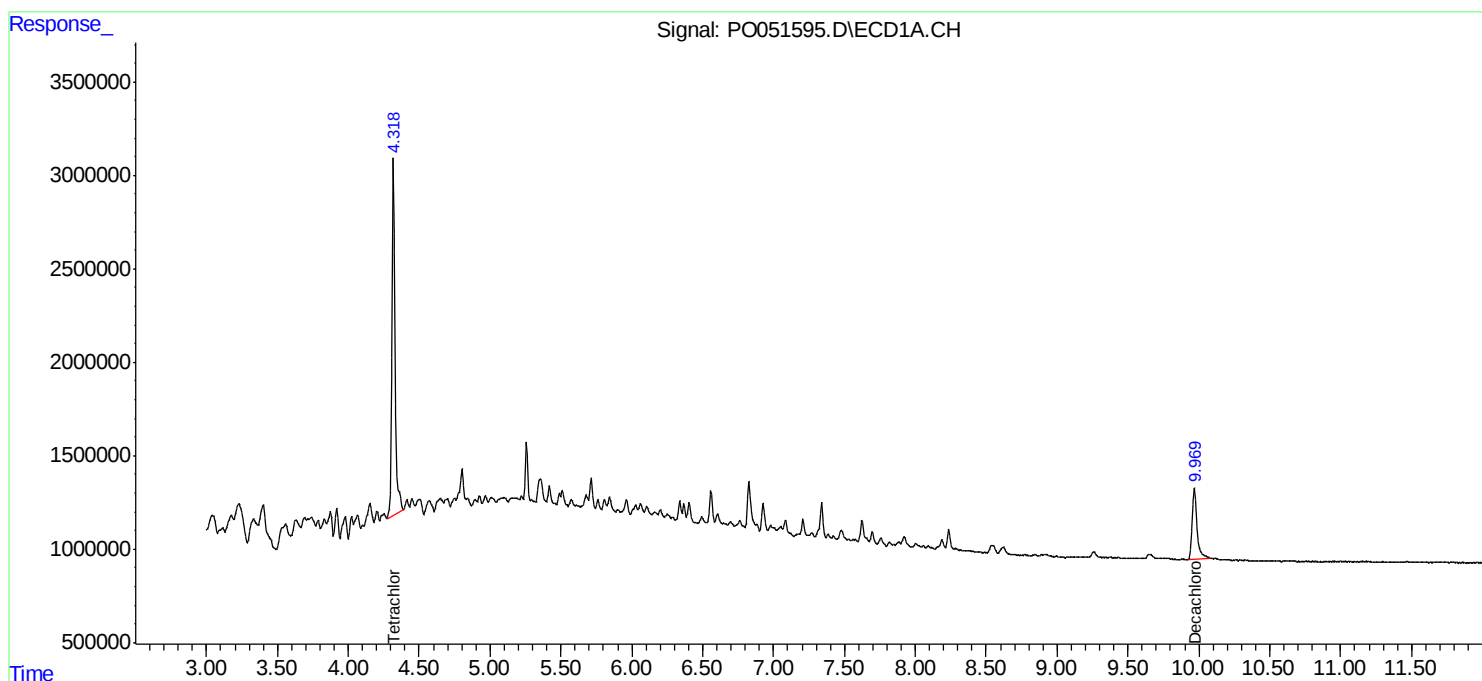

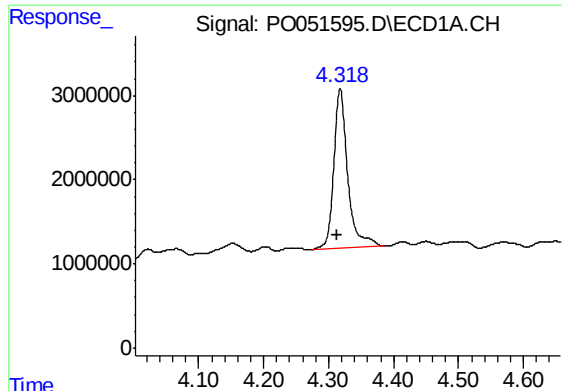


#1 Tetrachloro-m-xylene

R.T.: 4.318 min
Delta R.T.: 0.005 min
Response: 28389063
Conc: 8.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
OILY-WATER


Manual Integrations
APPROVED

Sohil
11/19/2018 4:40:26 PM

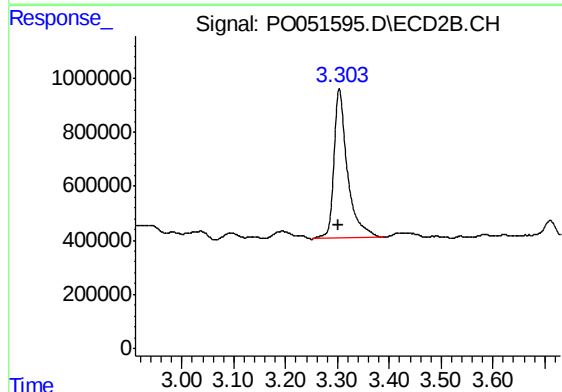


#1 Tetrachloro-m-xylene

R.T.: 3.304 min
Delta R.T.: 0.001 min
Response: 10132591
Conc: 9.20 ng/ml

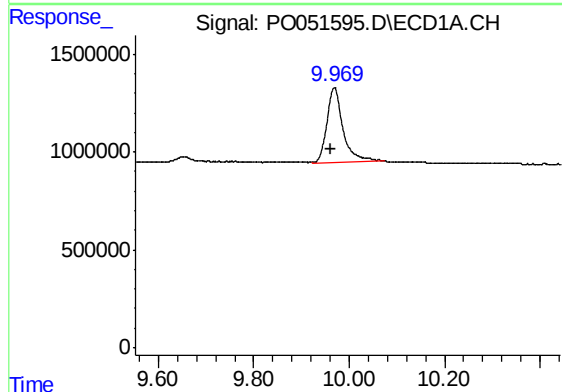

#2 Decachlorobiphenyl

R.T.: 9.969 min
Delta R.T.: 0.007 min
Response: 8976422
Conc: 4.68 ng/ml m

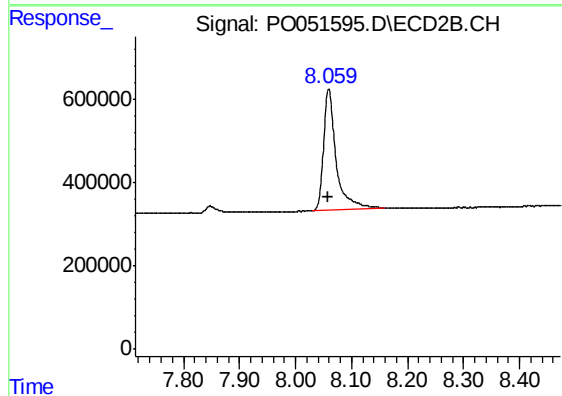

#2 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: 0.000 min
Response: 4571686
Conc: 5.52 ng/ml m