

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111618\
 Data File : P0051601.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Nov 2018 12:31
 Operator : SM/SJ
 Sample : J5767-15RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-01-111418-DRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 13:25:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 15 08:04:19 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.307	3.297	38739664	13277309	12.130	12.058
2) SA Decachlor...	9.955	8.054	18519284	7142271	9.649	8.616

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111618\
Data File : PO051601.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Nov 2018 12:31
Operator : SM/SJ
Sample : J5767-15RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-01-111418-DRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 13:25:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111318.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 15 08:04:19 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

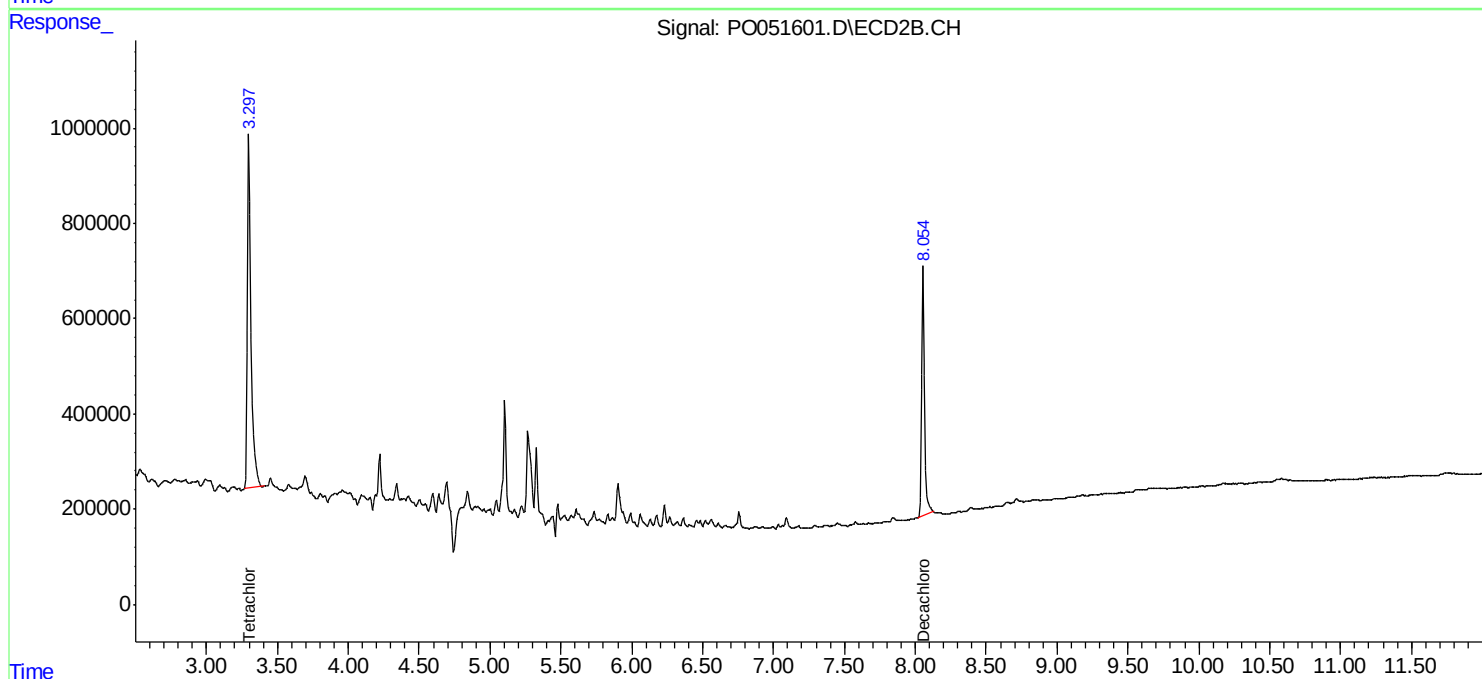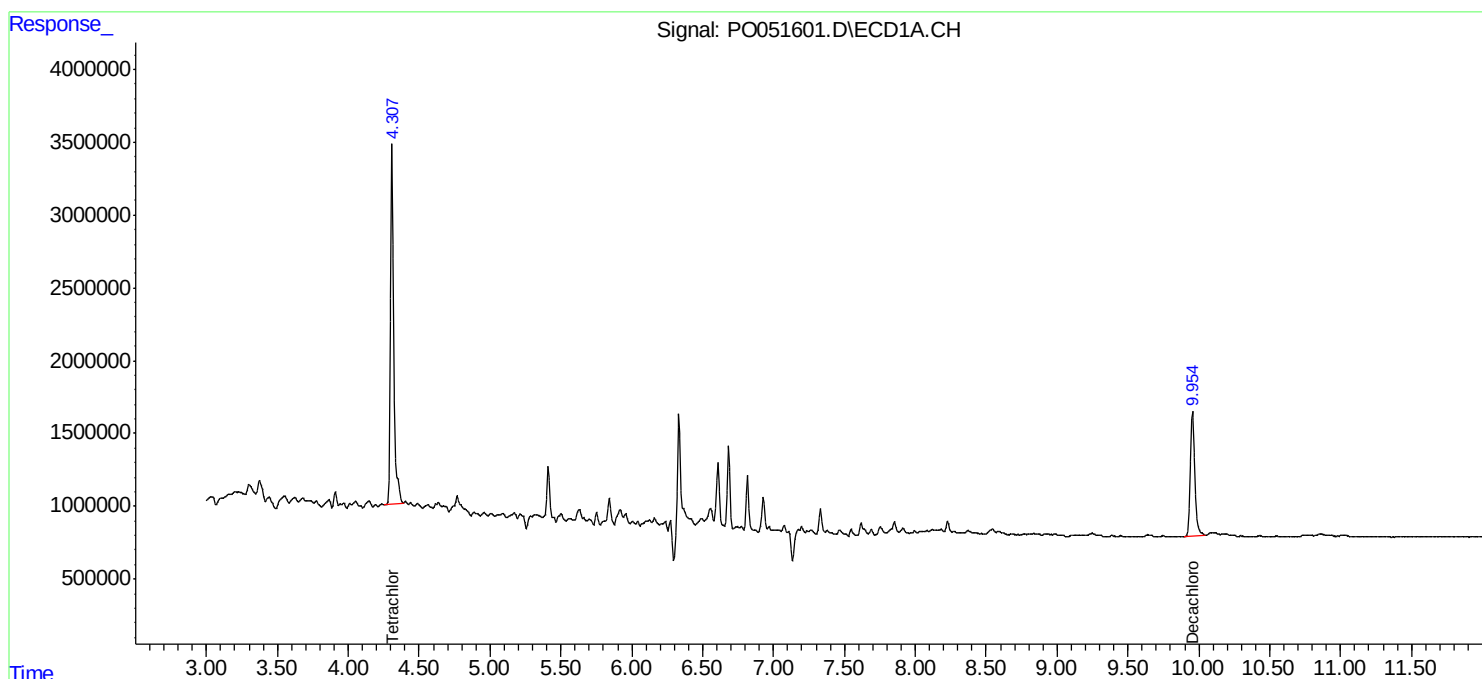


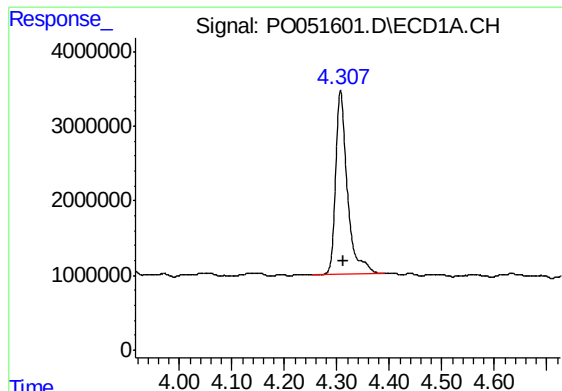

#1 Tetrachloro-m-xylene


R.T.: 4.307 min
Delta R.T.: -0.006 min
Response: 38739664
Conc: 12.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-01-111418-DRE

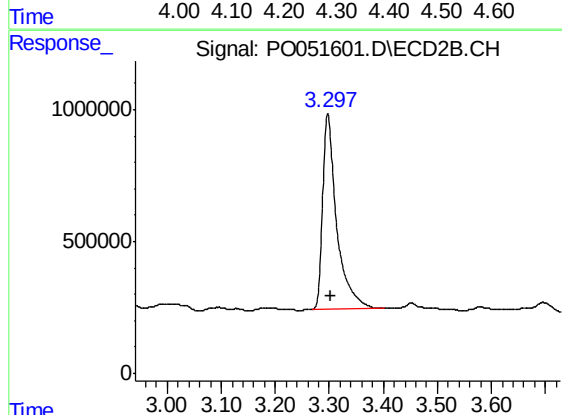


#1 Tetrachloro-m-xylene

R.T.: 3.297 min
Delta R.T.: -0.005 min
Response: 13277309
Conc: 12.06 ng/ml

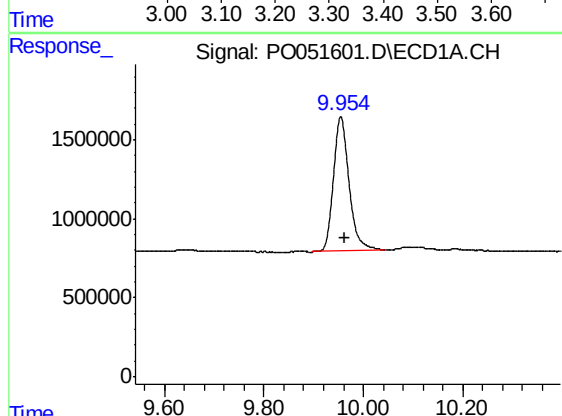

#2 Decachlorobiphenyl

R.T.: 9.955 min
Delta R.T.: -0.007 min
Response: 18519284
Conc: 9.65 ng/ml

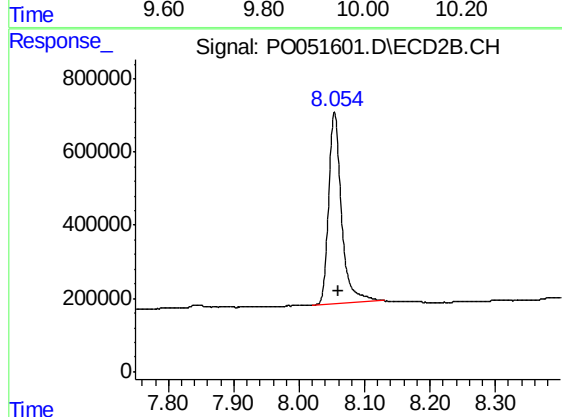

#2 Decachlorobiphenyl

R.T.: 8.054 min
Delta R.T.: -0.005 min
Response: 7142271
Conc: 8.62 ng/ml