

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111621\
 Data File : PO082969.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Nov 2021 17:29
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 00:54:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.960	3.959	1863561	658535	20.899	20.295
2)	SA Decachlor...	11.056	9.268	1355116	565981	23.399	19.962
Target Compounds							
8)	L2 AR-1221-1	5.201f	0.000	44499	0	45.495	N.D. #
9)	L2 AR-1221-2	5.315	0.000	25451	0	36.955	N.D. #
10)	L2 AR-1221-3	0.000	4.404	0	23512	N.D.	23.773 #
11)	L3 AR-1232-1	0.000	4.404	0	23512	N.D.	29.026 #
24)	L5 AR-1248-4	7.247	0.000	470	0	0.179	N.D. #
26)	L6 AR-1254-1	7.213	0.000	7397	0	2.646	N.D. #
28)	L6 AR-1254-3	7.843	0.000	51166	0	12.026	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111621\
Data File : PO082969.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Nov 2021 17:29
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 00:54:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

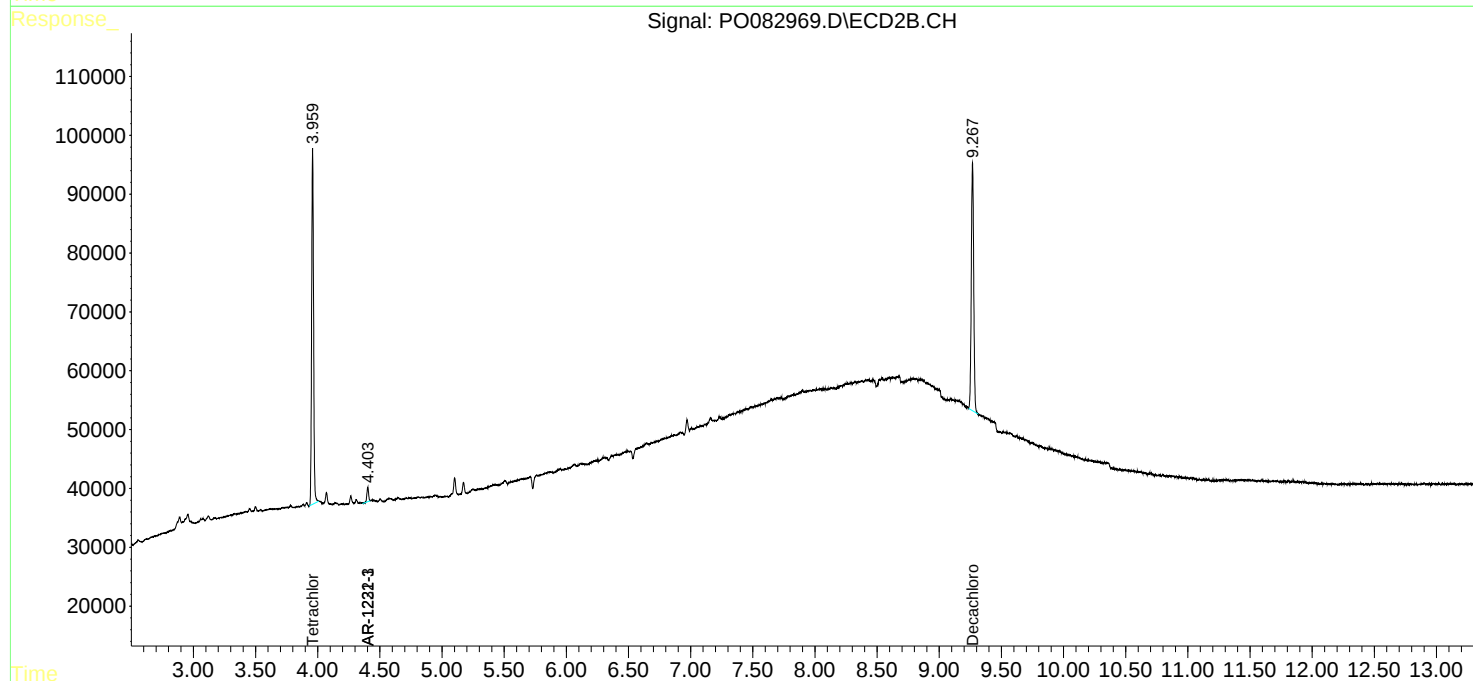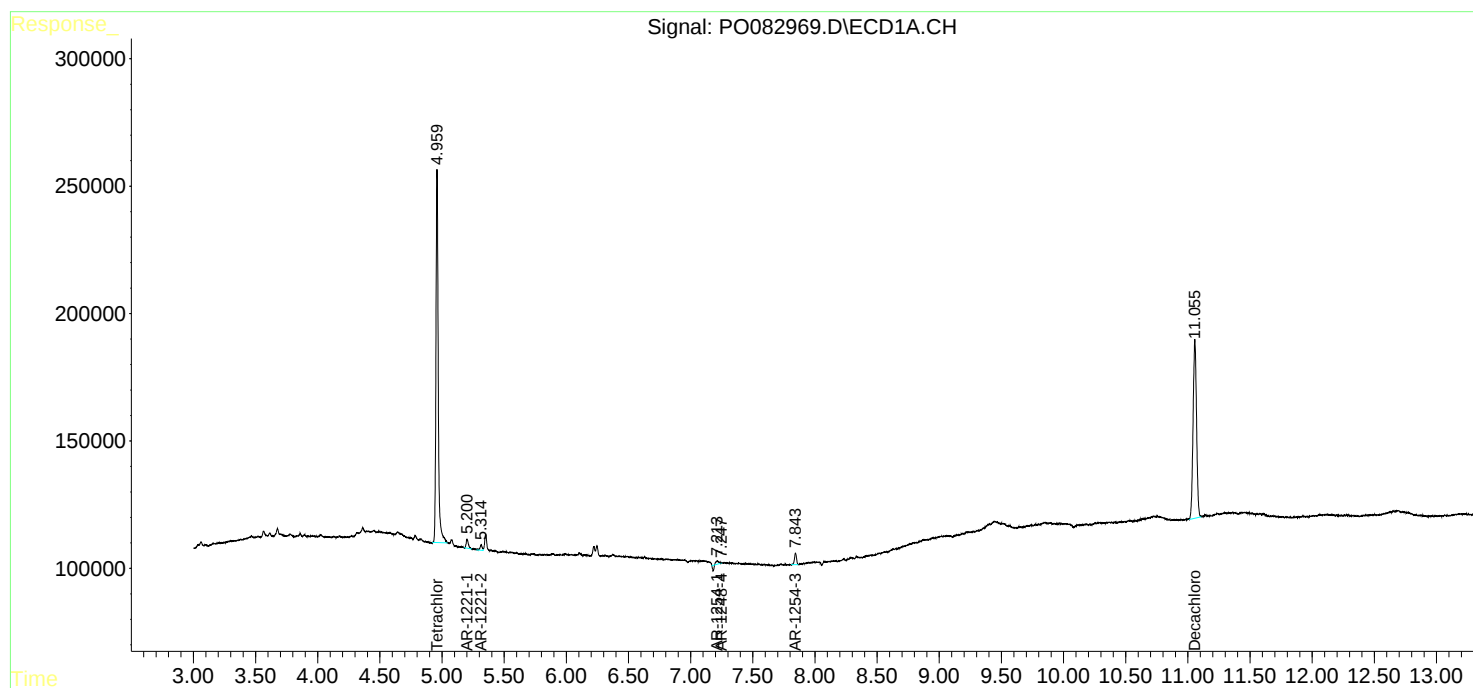


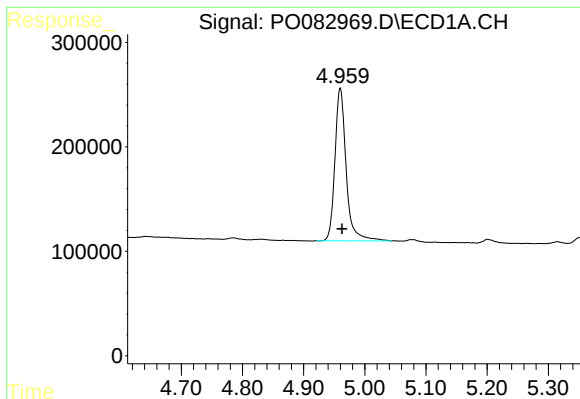

#1 Tetrachloro-m-xylene


R.T.: 4.960 min
Delta R.T.: -0.003 min
Response: 1863561
Conc: 20.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

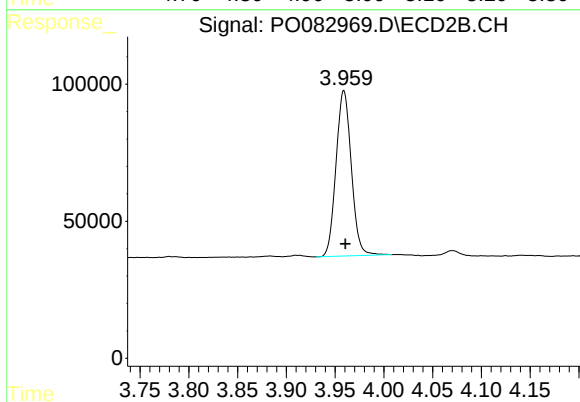


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: -0.002 min
Response: 658535
Conc: 20.29 ng/ml

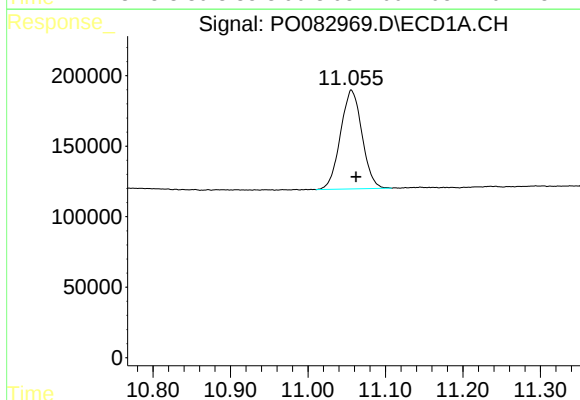


#2 Decachlorobiphenyl

R.T.: 11.056 min
Delta R.T.: -0.006 min
Response: 1355116
Conc: 23.40 ng/ml

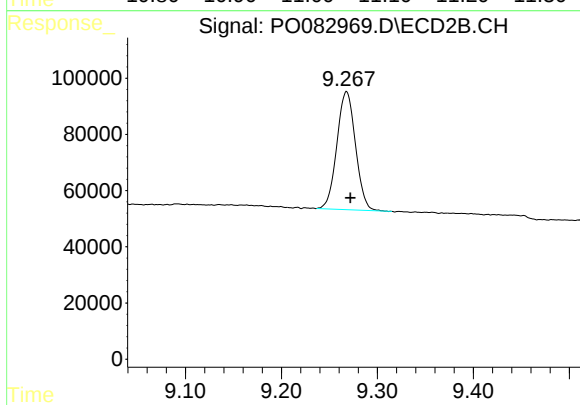

#2 Decachlorobiphenyl


R.T.: 9.268 min
Delta R.T.: -0.004 min
Response: 565981
Conc: 19.96 ng/ml

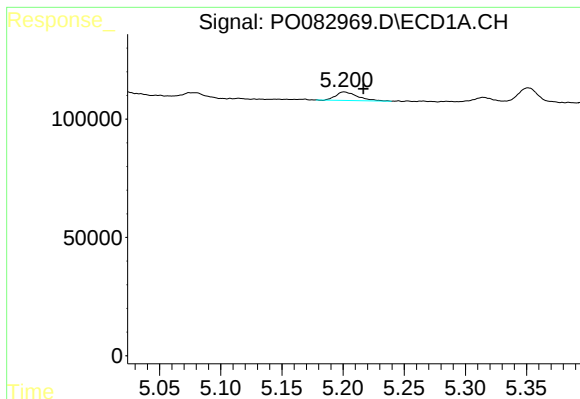

#8 AR-1221-1


R.T.: 5.201 min
Delta R.T.: -0.016 min
Response: 44499
Conc: 45.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

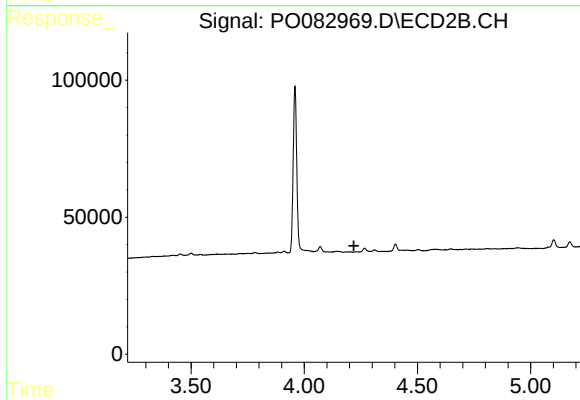


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.219 min
Response: 0
Conc: N.D.

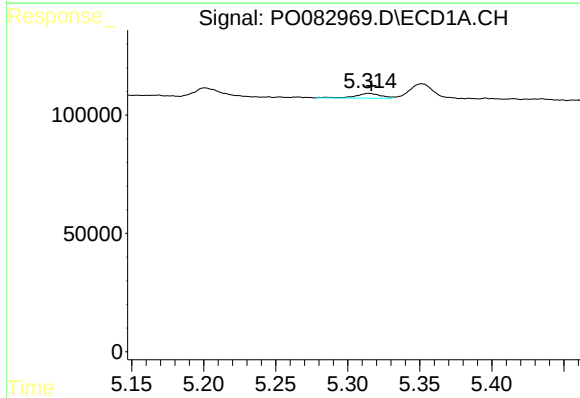


#9 AR-1221-2

R.T.: 5.315 min
Delta R.T.: -0.002 min
Response: 25451
Conc: 36.96 ng/ml

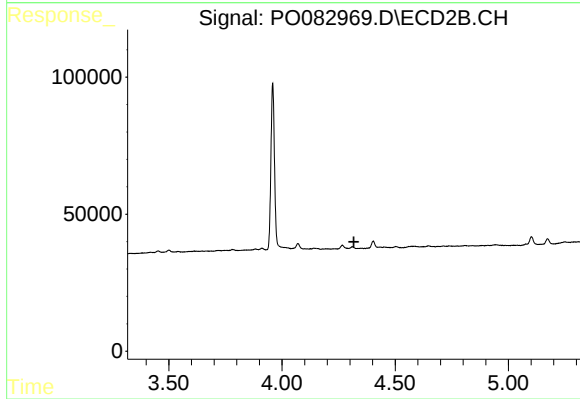

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

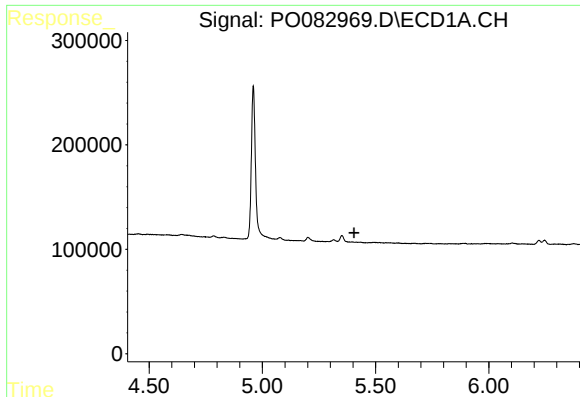

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

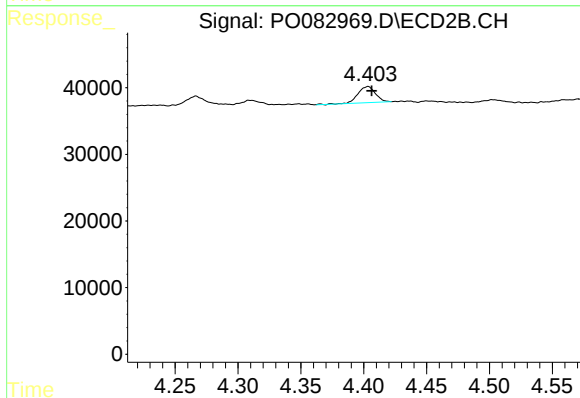


#10 AR-1221-3

R.T.: 4.404 min
Delta R.T.: -0.003 min
Response: 23512
Conc: 23.77 ng/ml

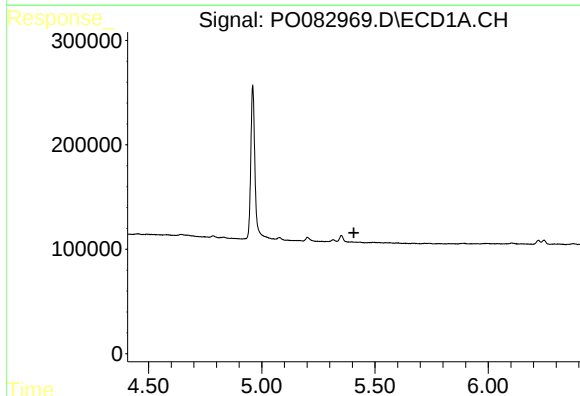


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

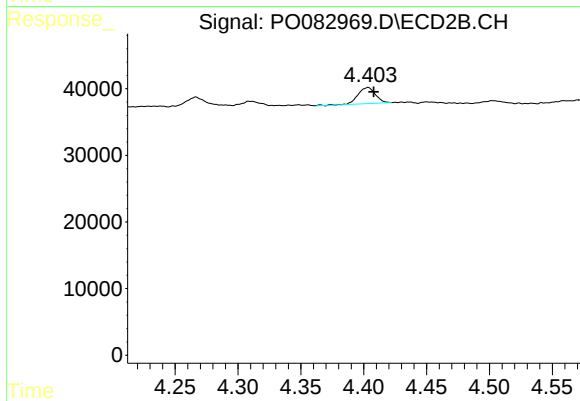

#11 AR-1232-1


R.T.: 4.404 min
Delta R.T.: -0.004 min
Response: 23512
Conc: 29.03 ng/ml

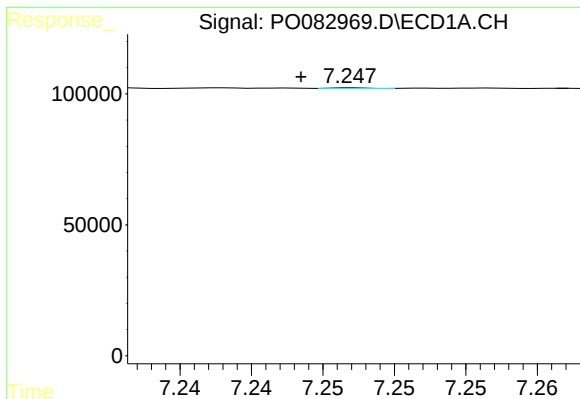

#24 AR-1248-4


R.T.: 7.247 min
Delta R.T.: 0.004 min
Response: 470
Conc: 0.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

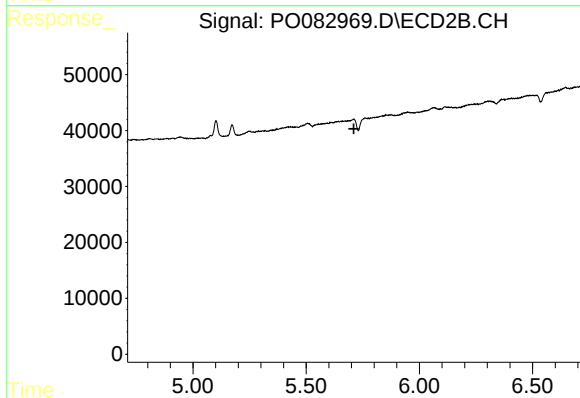


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.711 min
Response: 0
Conc: N.D.

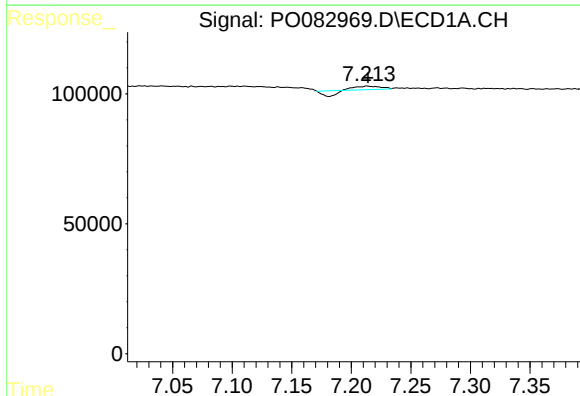


#26 AR-1254-1

R.T.: 7.213 min
Delta R.T.: 0.000 min
Response: 7397
Conc: 2.65 ng/ml

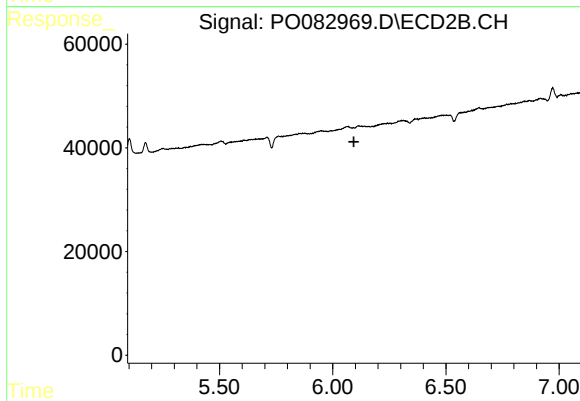

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

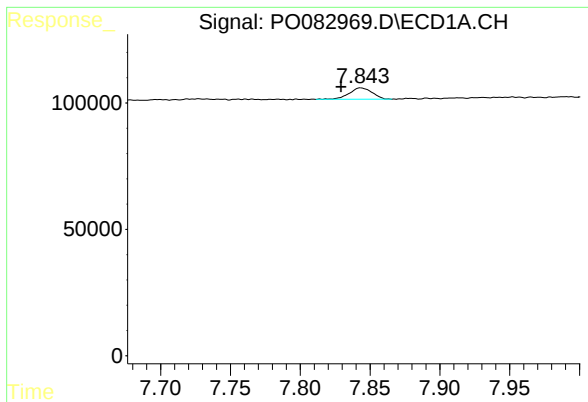

#28 AR-1254-3

R.T.: 7.843 min
Delta R.T.: 0.014 min
Response: 51166
Conc: 12.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

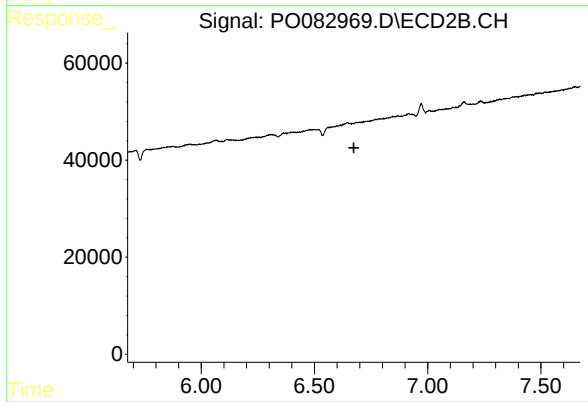

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.674 min
Response: 0
Conc: N.D.