

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111622\
 Data File : PO090641.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 13:27
 Operator : YP/AJ
 Sample : PB149096BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB149096BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/17/2022
 Supervised By :Ankita Jodhani 11/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 20:30:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.303	3.479	76620226	23690443	23.840	22.291m
2) SA Decachlor...	10.062	8.488	63271063	24548418	25.819	23.835

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111622\
Data File : PO090641.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 13:27
Operator : YP/AJ
Sample : PB149096BL
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB149096BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/17/2022
Supervised By :Ankita Jodhani 11/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 20:30:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

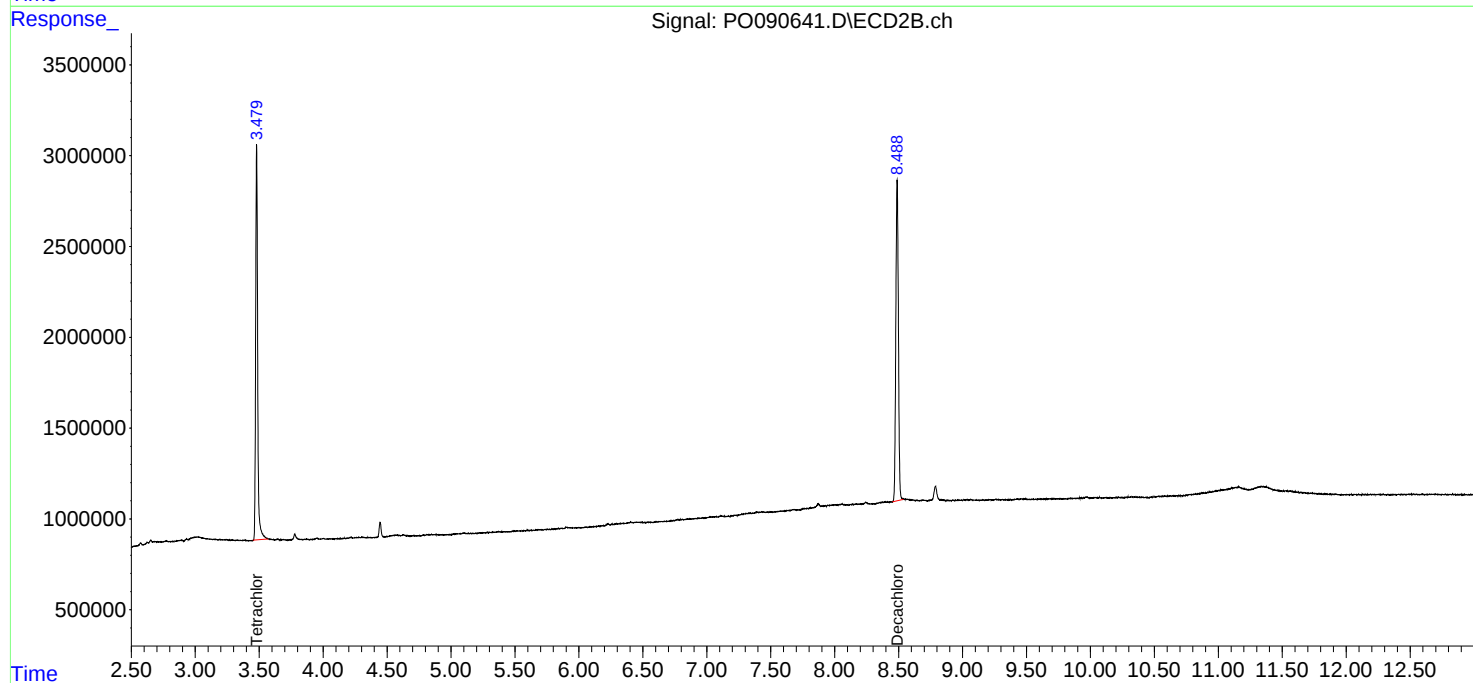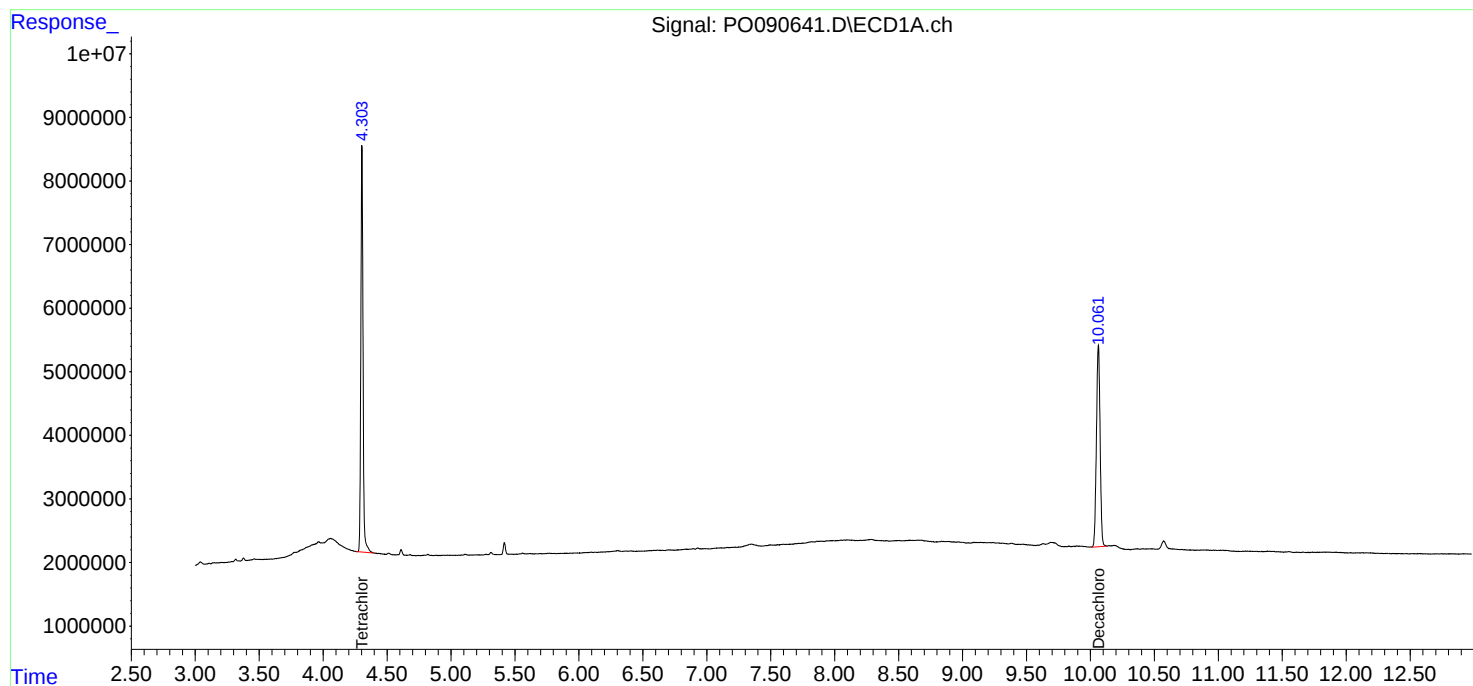

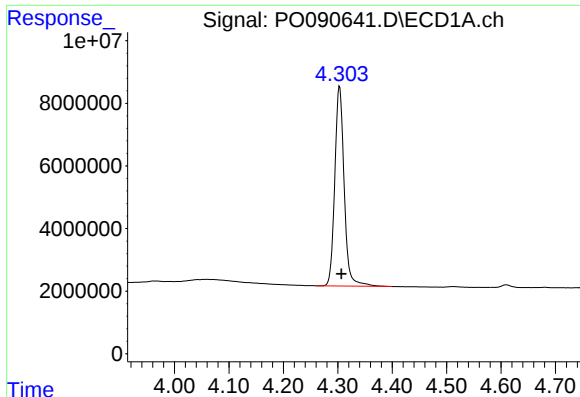


#1 Tetrachloro-m-xylene

R.T.: 4.303 min
Delta R.T.: -0.004 min
Response: 76620226
Conc: 23.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB149096BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/17/2022
Supervised By :Ankita Jodhani 11/17/2022

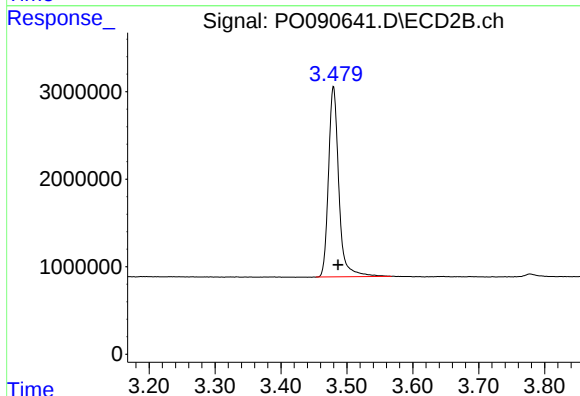


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: -0.007 min
Response: 23690443
Conc: 22.29 ng/ml m

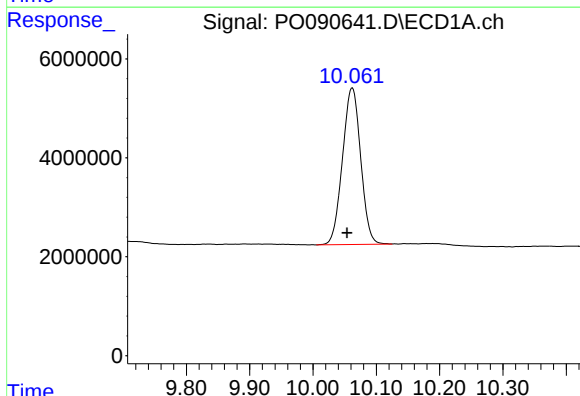

#2 Decachlorobiphenyl

R.T.: 10.062 min
Delta R.T.: 0.008 min
Response: 63271063
Conc: 25.82 ng/ml

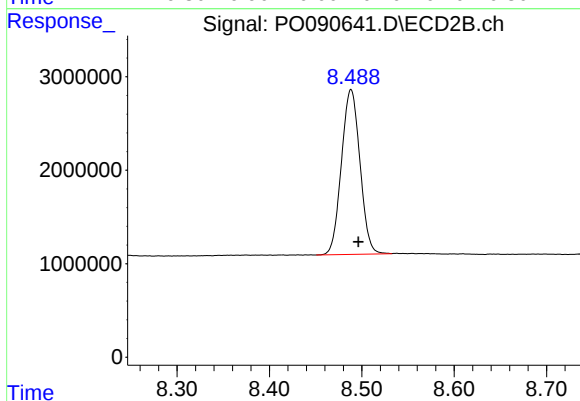

#2 Decachlorobiphenyl

R.T.: 8.488 min
Delta R.T.: -0.008 min
Response: 24548418
Conc: 23.84 ng/ml