

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111622\
 Data File : P0090648.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 15:26
 Operator : YP/AJ
 Sample : N5632-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MLMR-SILICA-115

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/17/2022
 Supervised By :Ankita Jodhani 11/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 20:33:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.303	3.480	32602806	18286393	10.144	17.206m#
2) SA Decachlor...	10.056	8.488	54104138	21651729	22.078	21.023

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111622\
Data File : PO090648.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 15:26
Operator : YP/AJ
Sample : N5632-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MLMR-SILICA-115


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/17/2022
Supervised By :Ankita Jodhani 11/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 20:33:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

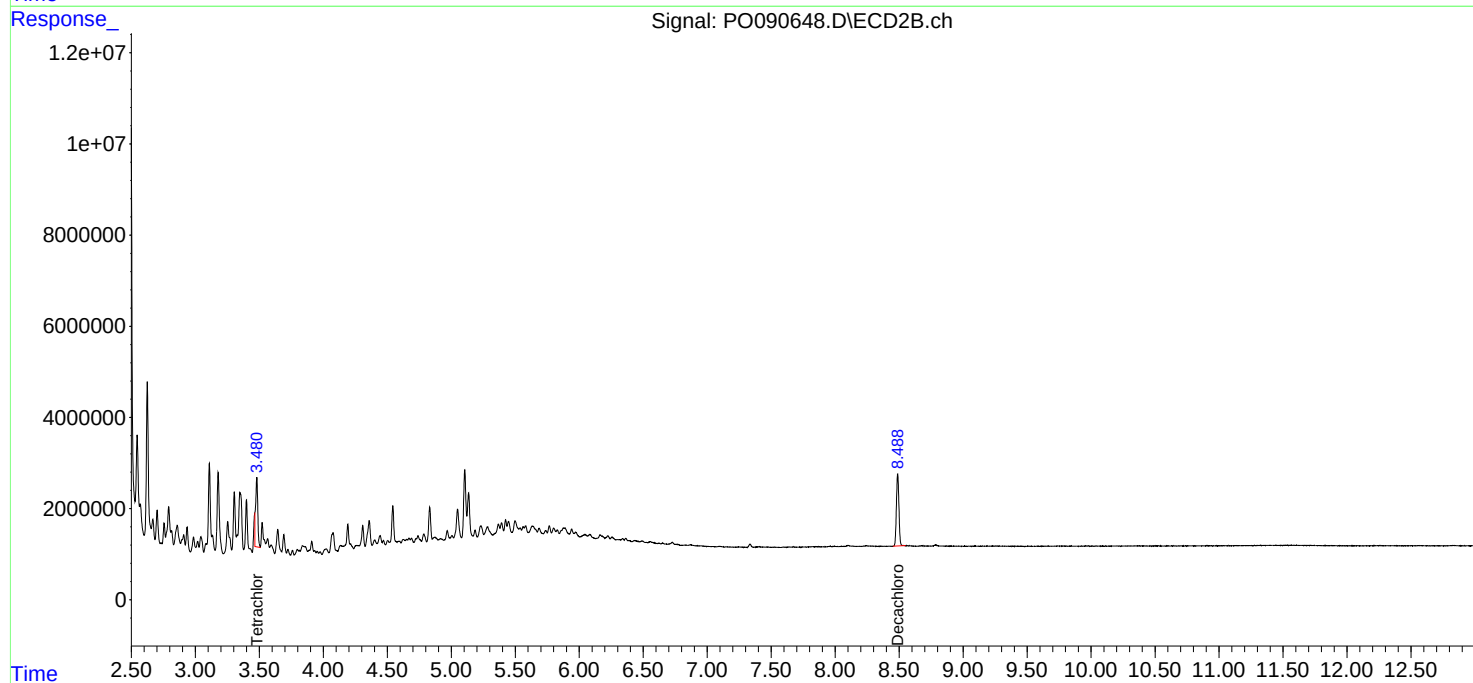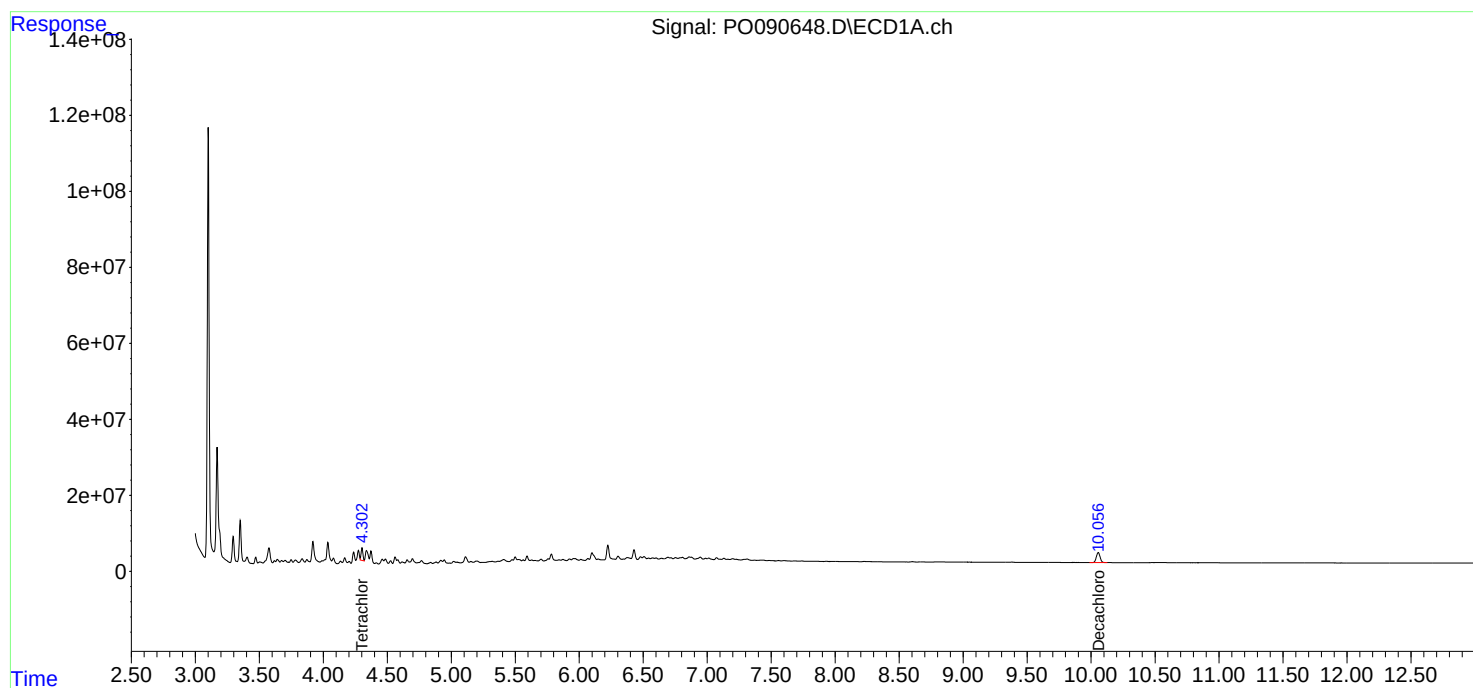

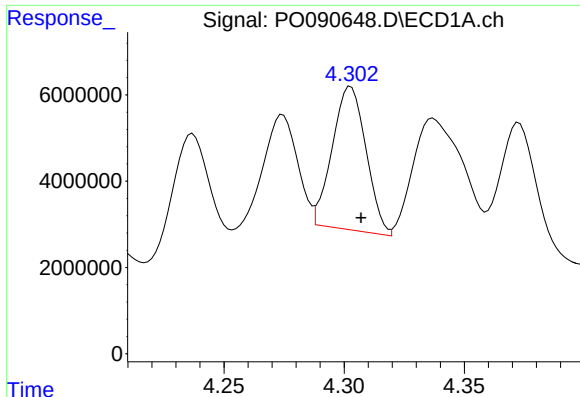


#1 Tetrachloro-m-xylene

R.T.: 4.303 min
Delta R.T.: -0.004 min
Response: 32602806
Conc: 10.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
MLMR-SILICA-115


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/17/2022
Supervised By :Ankita Jodhani 11/17/2022

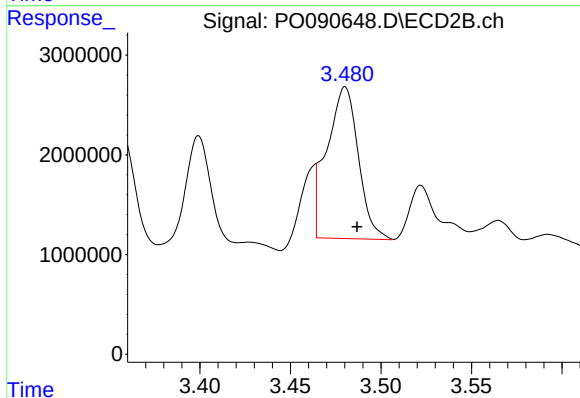


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: -0.007 min
Response: 18286393
Conc: 17.21 ng/ml m

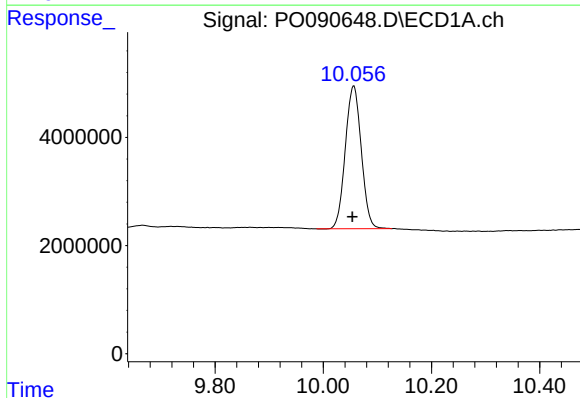

#2 Decachlorobiphenyl

R.T.: 10.056 min
Delta R.T.: 0.003 min
Response: 54104138
Conc: 22.08 ng/ml

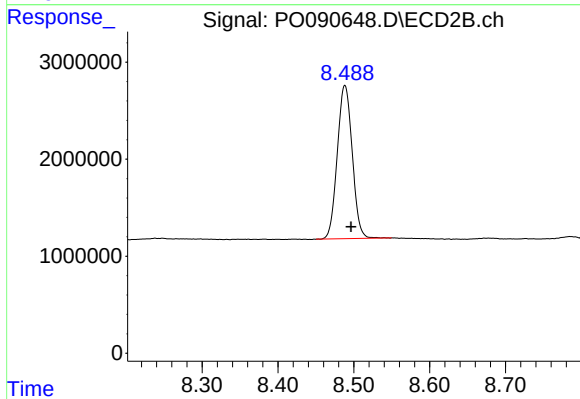

#2 Decachlorobiphenyl

R.T.: 8.488 min
Delta R.T.: -0.008 min
Response: 21651729
Conc: 21.02 ng/ml