

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111720\
 Data File : PO073275.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Nov 2020 20:01
 Operator : DD\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Ankita
 11/18/2020 10:24:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 04:34:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 04:01:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.945	4.015	331043	198610	5.089	5.404
2)	SA Decachlor...	10.973	9.290	355582	230419	5.801	5.892
Target Compounds							
26)	L6 AR-1254-1	7.181	6.134	178218	142599	60.518	57.987
27)	L6 AR-1254-2	7.412	6.293	292791	128354	61.465	58.705
28)	L6 AR-1254-3	7.794	6.710	271654	218022	56.815	60.153m
29)	L6 AR-1254-4	8.091	6.949	269163	144037	63.056	60.232
30)	L6 AR-1254-5	8.521	7.376	235160	201348	58.909	60.748

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111720\
Data File : PO073275.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2020 20:01
Operator : DD\AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
11/18/2020 10:24:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:34:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 04:01:14 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

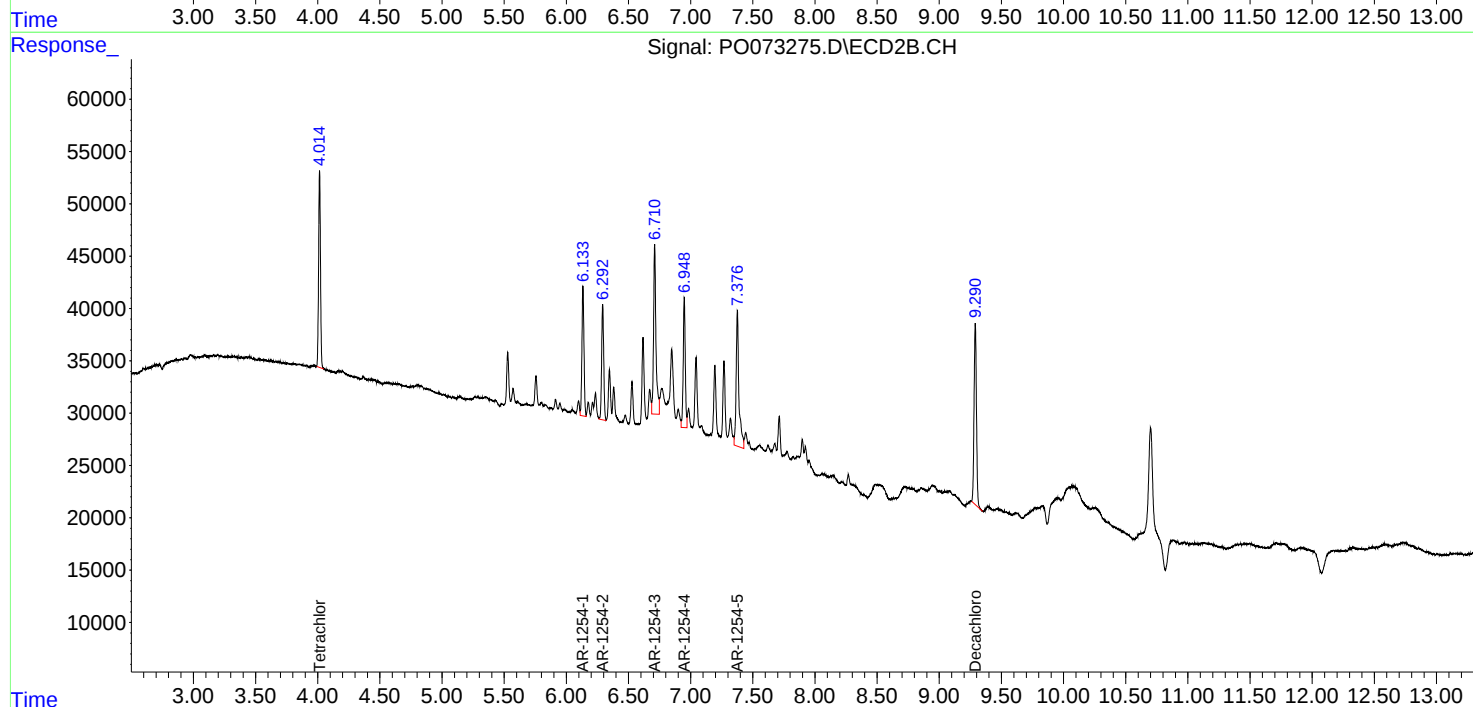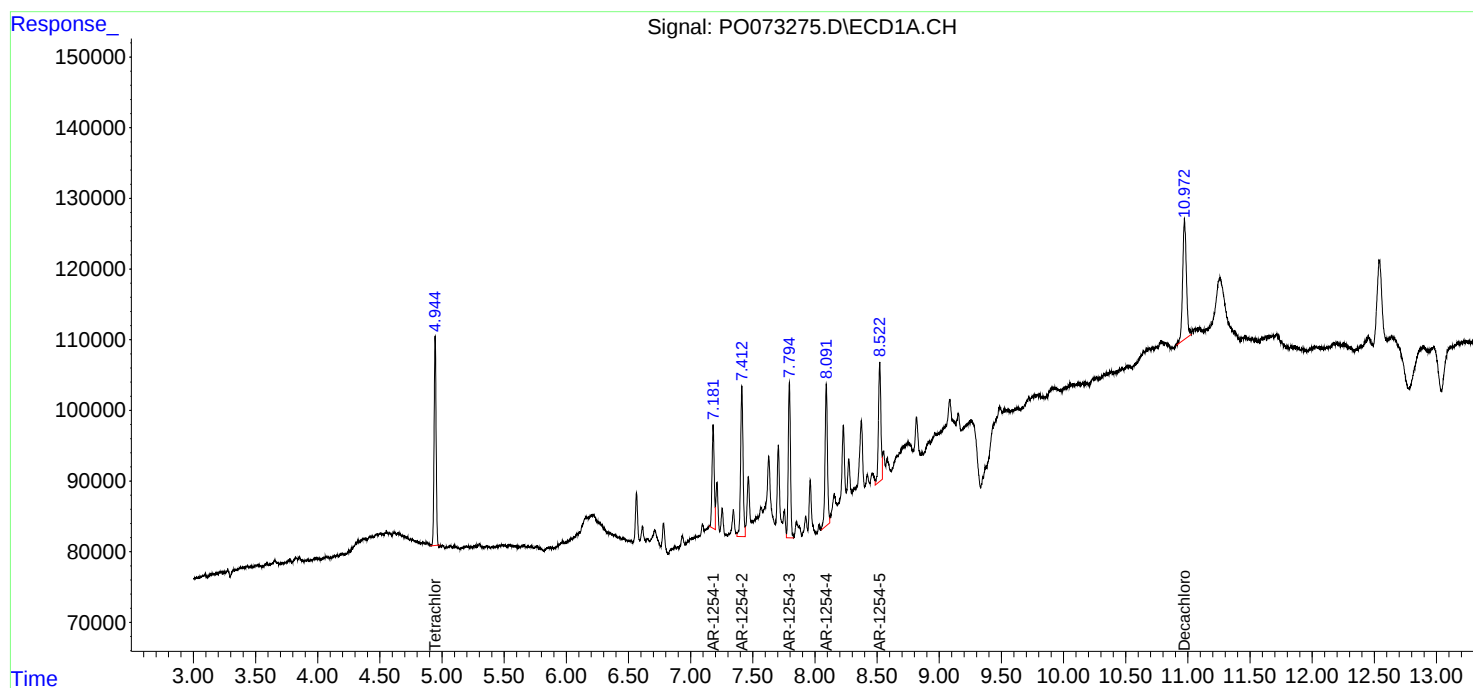

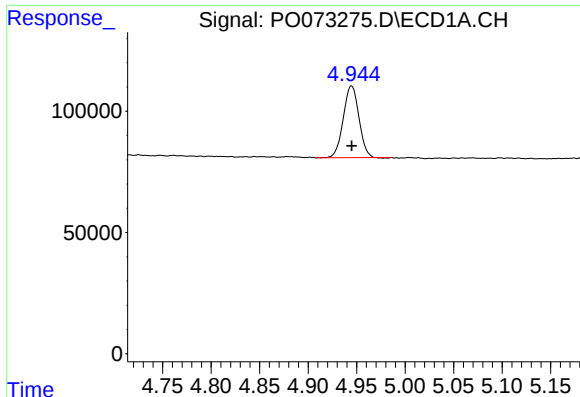


#1 Tetrachloro-m-xylene

R.T.: 4.945 min
Delta R.T.: 0.000 min
Response: 331043
Conc: 5.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
11/18/2020 10:24:09 AM

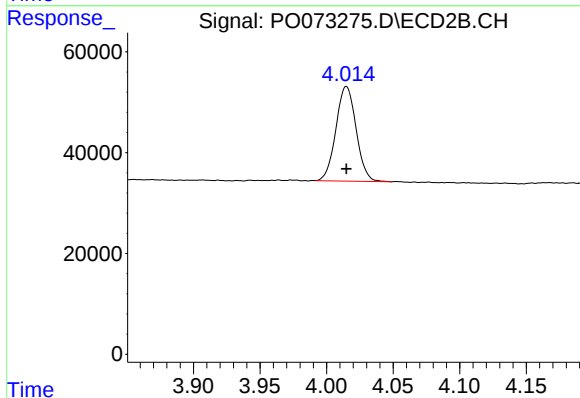


#1 Tetrachloro-m-xylene

R.T.: 4.015 min
Delta R.T.: 0.000 min
Response: 198610
Conc: 5.40 ng/ml

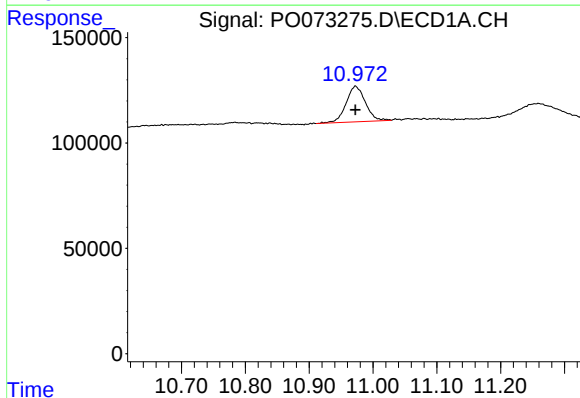


#2 Decachlorobiphenyl

R.T.: 10.973 min
Delta R.T.: 0.000 min
Response: 355582
Conc: 5.80 ng/ml

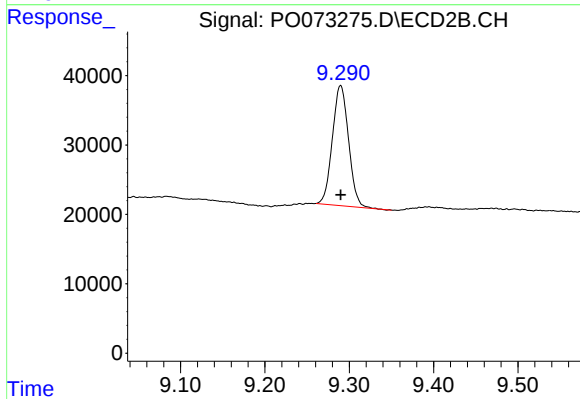

#2 Decachlorobiphenyl

R.T.: 9.290 min
Delta R.T.: 0.000 min
Response: 230419
Conc: 5.89 ng/ml

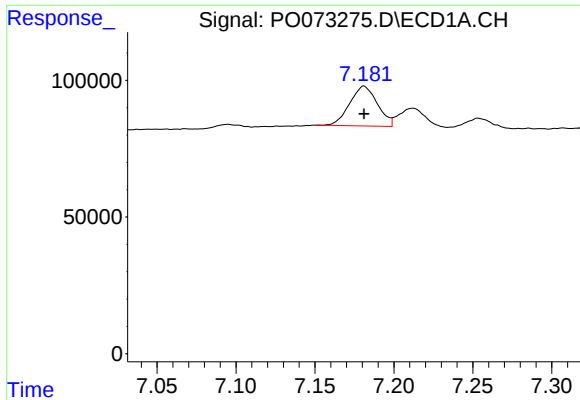


#26 AR-1254-1

R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 178218
Conc: 60.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Ankita
11/18/2020 10:24:09 AM

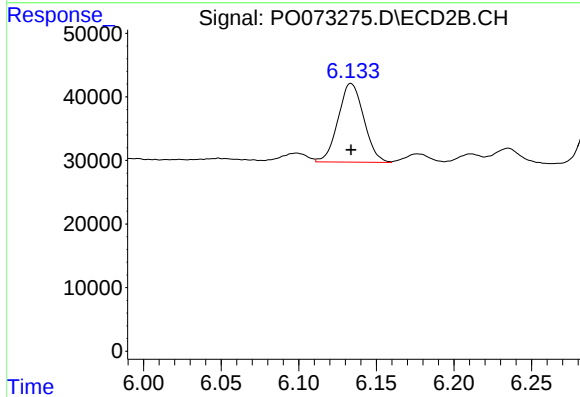


#26 AR-1254-1

R.T.: 6.134 min
Delta R.T.: 0.000 min
Response: 142599
Conc: 57.99 ng/ml

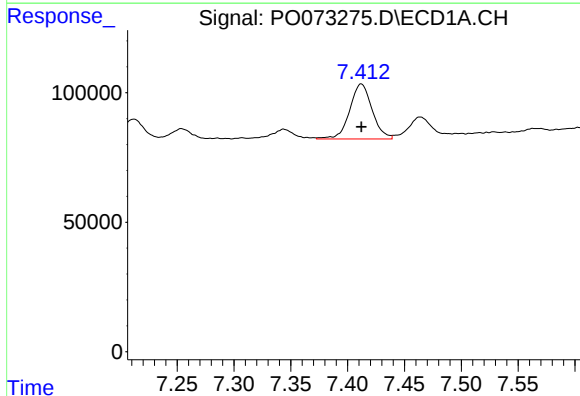


#27 AR-1254-2

R.T.: 7.412 min
Delta R.T.: 0.000 min
Response: 292791
Conc: 61.46 ng/ml

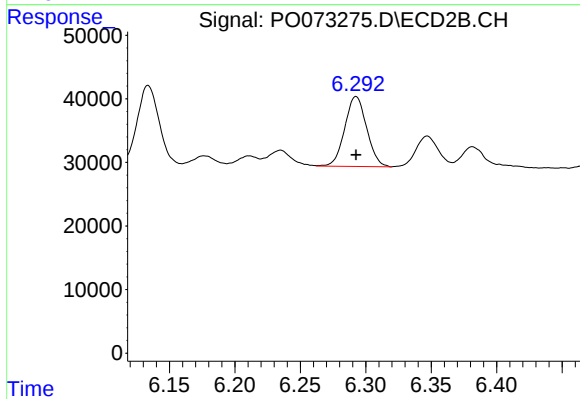

#27 AR-1254-2

R.T.: 6.293 min
Delta R.T.: 0.000 min
Response: 128354
Conc: 58.71 ng/ml

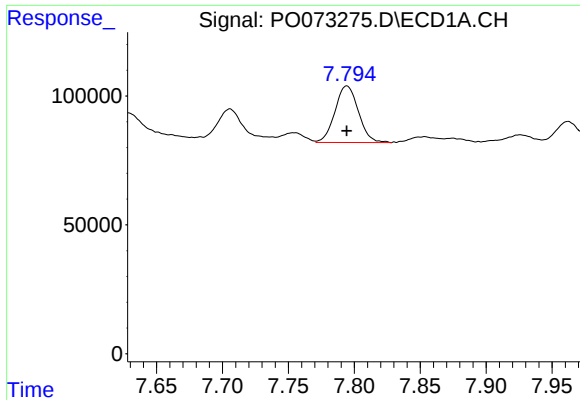


#28 AR-1254-3

R.T.: 7.794 min
Delta R.T.: 0.000 min
Response: 271654
Conc: 56.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254\ICC050


Manual Integrations
APPROVED

Ankita
11/18/2020 10:24:09 AM

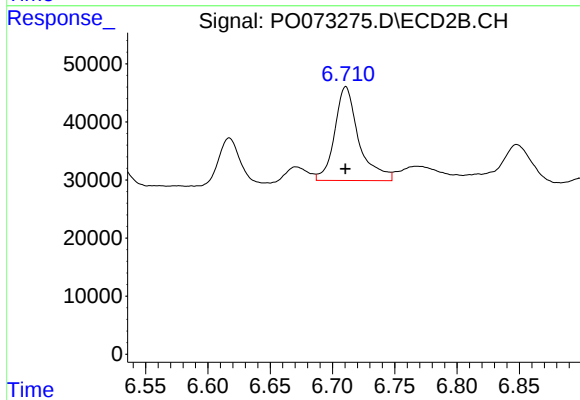


#28 AR-1254-3

R.T.: 6.710 min
Delta R.T.: 0.000 min
Response: 218022
Conc: 60.15 ng/ml m

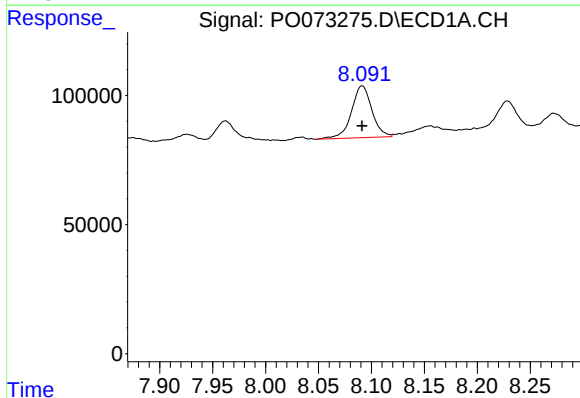


#29 AR-1254-4

R.T.: 8.091 min
Delta R.T.: 0.000 min
Response: 269163
Conc: 63.06 ng/ml

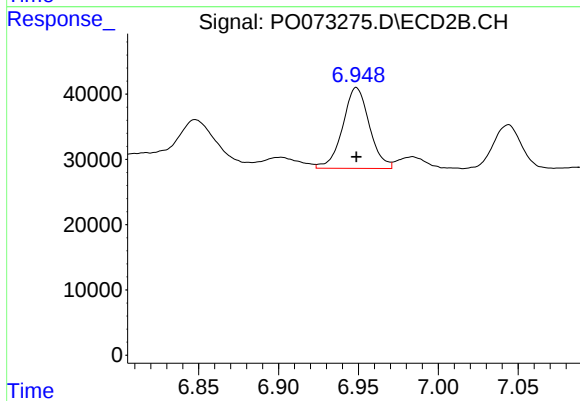

#29 AR-1254-4

R.T.: 6.949 min
Delta R.T.: 0.000 min
Response: 144037
Conc: 60.23 ng/ml

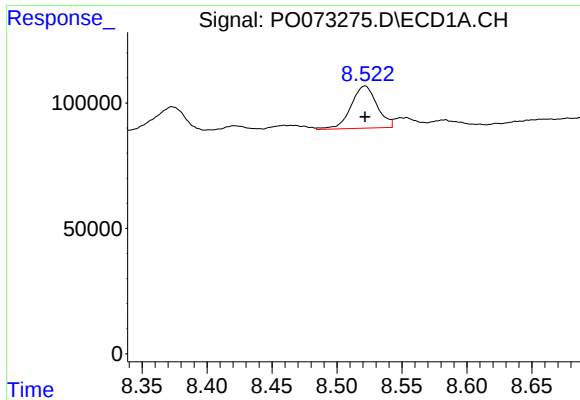


#30 AR-1254-5

R.T.: 8.521 min
Delta R.T.: 0.000 min
Response: 235160
Conc: 58.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Ankita
11/18/2020 10:24:09 AM

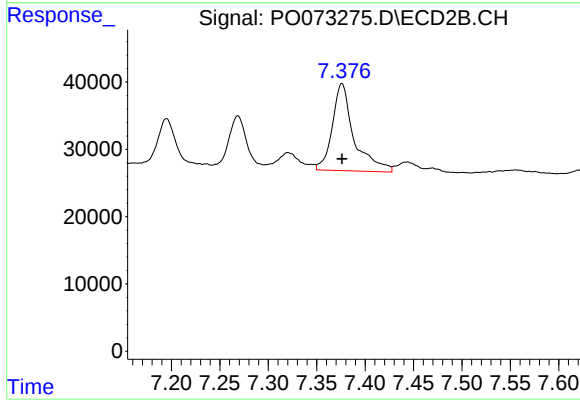

#30 AR-1254-5

R.T.: 7.376 min
Delta R.T.: 0.000 min
Response: 201348
Conc: 60.75 ng/ml