

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO111721\
 Data File : PO083010.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Nov 2021 22:09
 Operator : AJ\MA
 Sample : M4714-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 2ND-FLOOR-SLAB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 02:56:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.956	3.956	1992187	697818	22.341	21.505
2) SA Decachlor...	11.051	9.262	1474239	668331	25.455	23.572
Target Compounds						
8) L2 AR-1221-1	5.211	0.000	107179	0	109.579	N.D. #
9) L2 AR-1221-2	5.312	0.000	26343	0	38.250	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111721\
Data File : P0083010.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2021 22:09
Operator : AJ\MA
Sample : M4714-08
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2ND-FLOOR-SLAB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 02:56:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

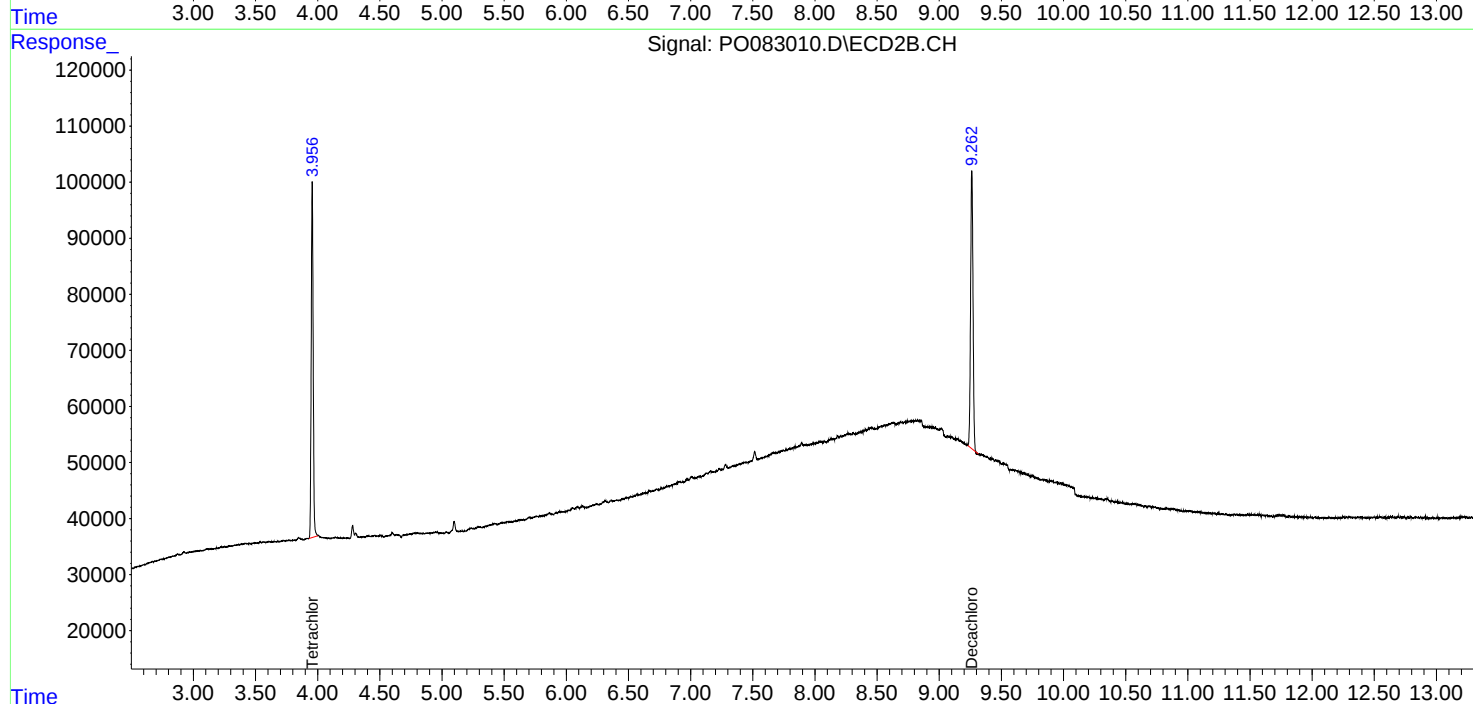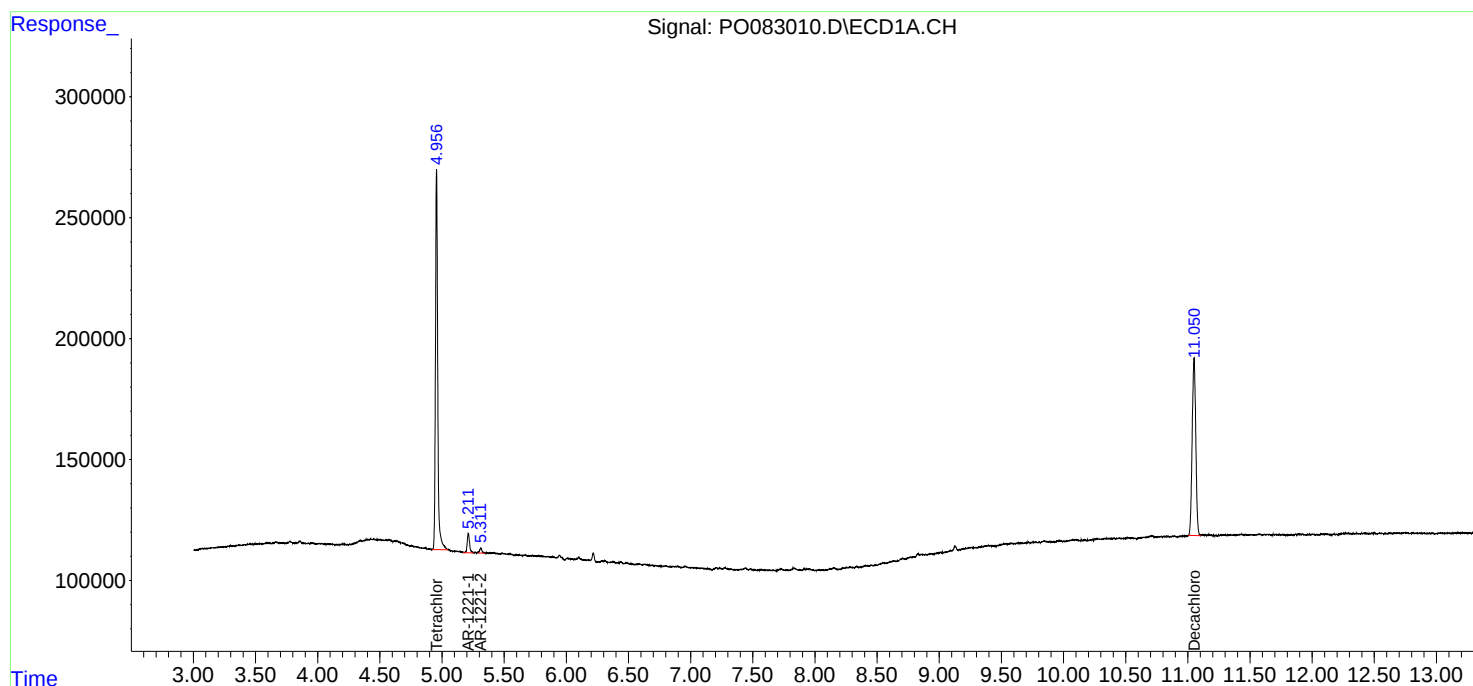


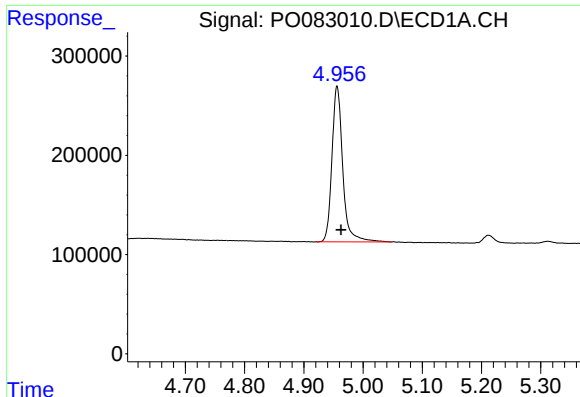

#1 Tetrachloro-m-xylene


R.T.: 4.956 min
Delta R.T.: -0.007 min
Response: 1992187
Conc: 22.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
2ND-FLOOR-SLAB

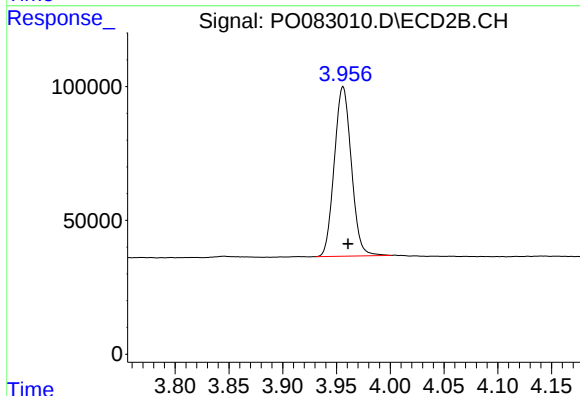


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.005 min
Response: 697818
Conc: 21.51 ng/ml

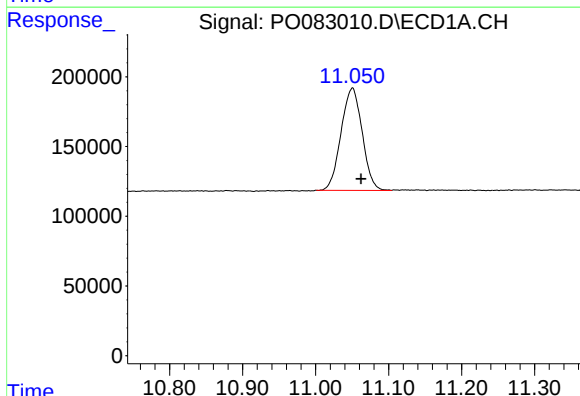


#2 Decachlorobiphenyl

R.T.: 11.051 min
Delta R.T.: -0.011 min
Response: 1474239
Conc: 25.46 ng/ml

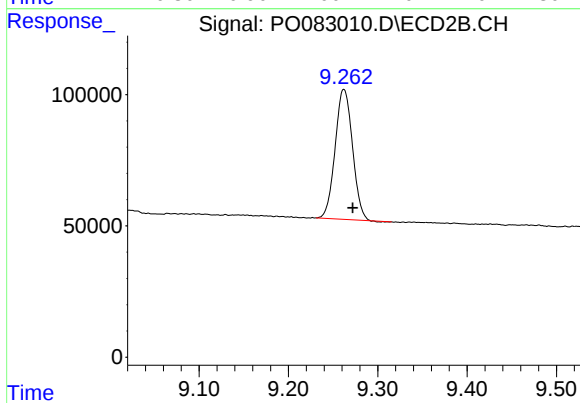

#2 Decachlorobiphenyl


R.T.: 9.262 min
Delta R.T.: -0.010 min
Response: 668331
Conc: 23.57 ng/ml

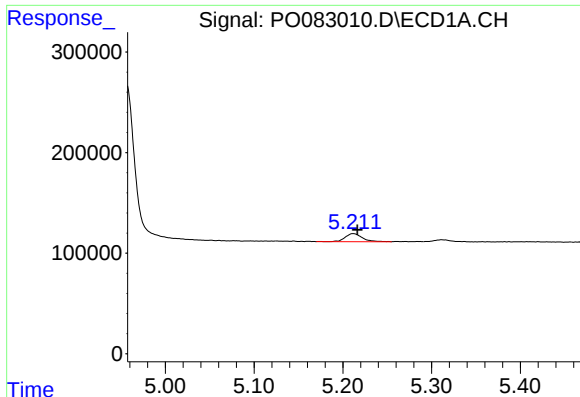

#8 AR-1221-1


R.T.: 5.211 min
Delta R.T.: -0.005 min
Response: 107179
Conc: 109.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
2ND-FLOOR-SLAB

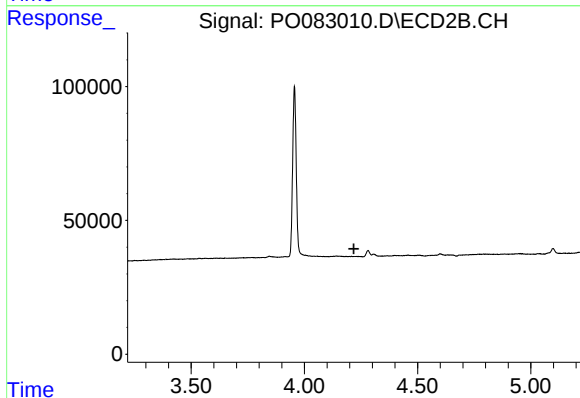


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.219 min
Response: 0
Conc: N.D.

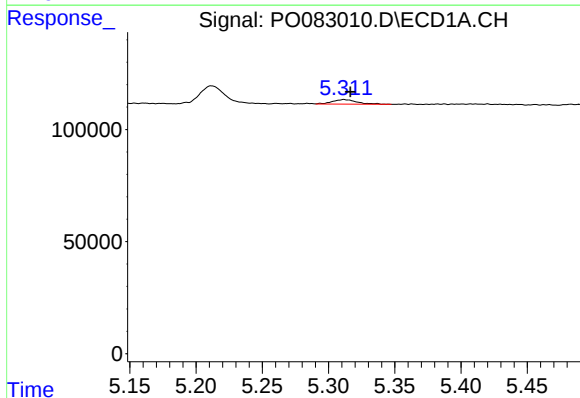

#9 AR-1221-2

R.T.: 5.312 min
Delta R.T.: -0.005 min
Response: 26343
Conc: 38.25 ng/ml

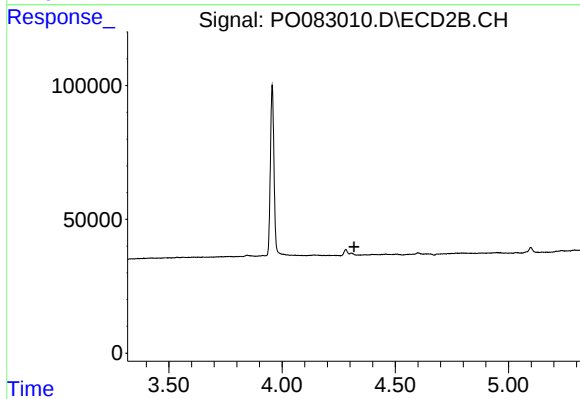

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.