

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111721\
 Data File : PO082999.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Nov 2021 18:25
 Operator : AJ\MA
 Sample : M4724-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FLOOR-1-ROOM-2-PILLARS

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
 Supervised By :mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 12:50:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.958	3.957	2032214	712002	22.790	21.942
2)	SA Decachlor...	11.050	9.264	1475725	670135	25.481	23.636
Target Compounds							
26)	L6 AR-1254-1	7.206	6.088	30904	21221	11.056	10.291
27)	L6 AR-1254-2	7.439	6.247	52988	11607	12.495	6.430m#
28)	L6 AR-1254-3	7.822	6.667	59789	35933	14.053	12.962
29)	L6 AR-1254-4	8.121	6.908	33717	22904	11.300	11.427
30)	L6 AR-1254-5	8.553	7.339	54719	29604	17.677	11.708 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO111721\
Data File : P0082999.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2021 18:25
Operator : AJ\MA
Sample : M4724-02
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_0
ClientSampleId :
FLOOR-1-ROOM-2-PILLARS


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 12:50:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

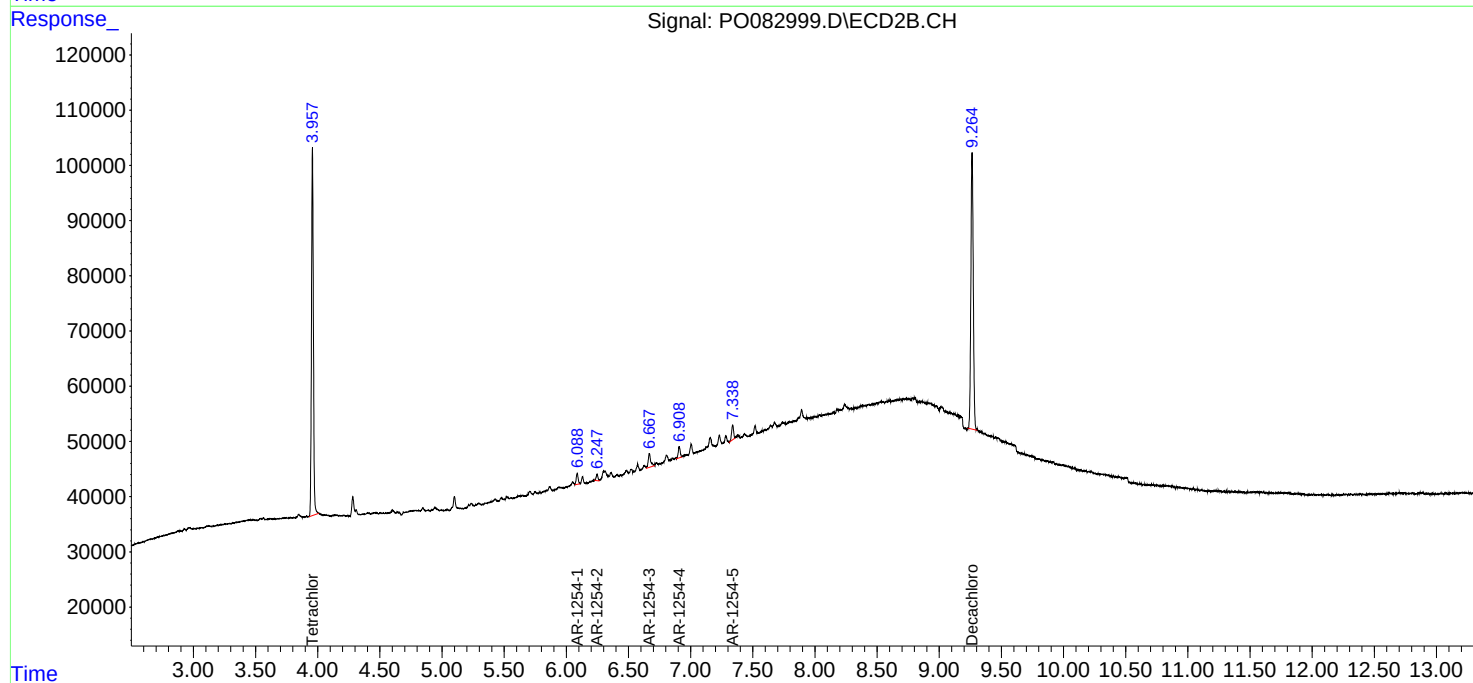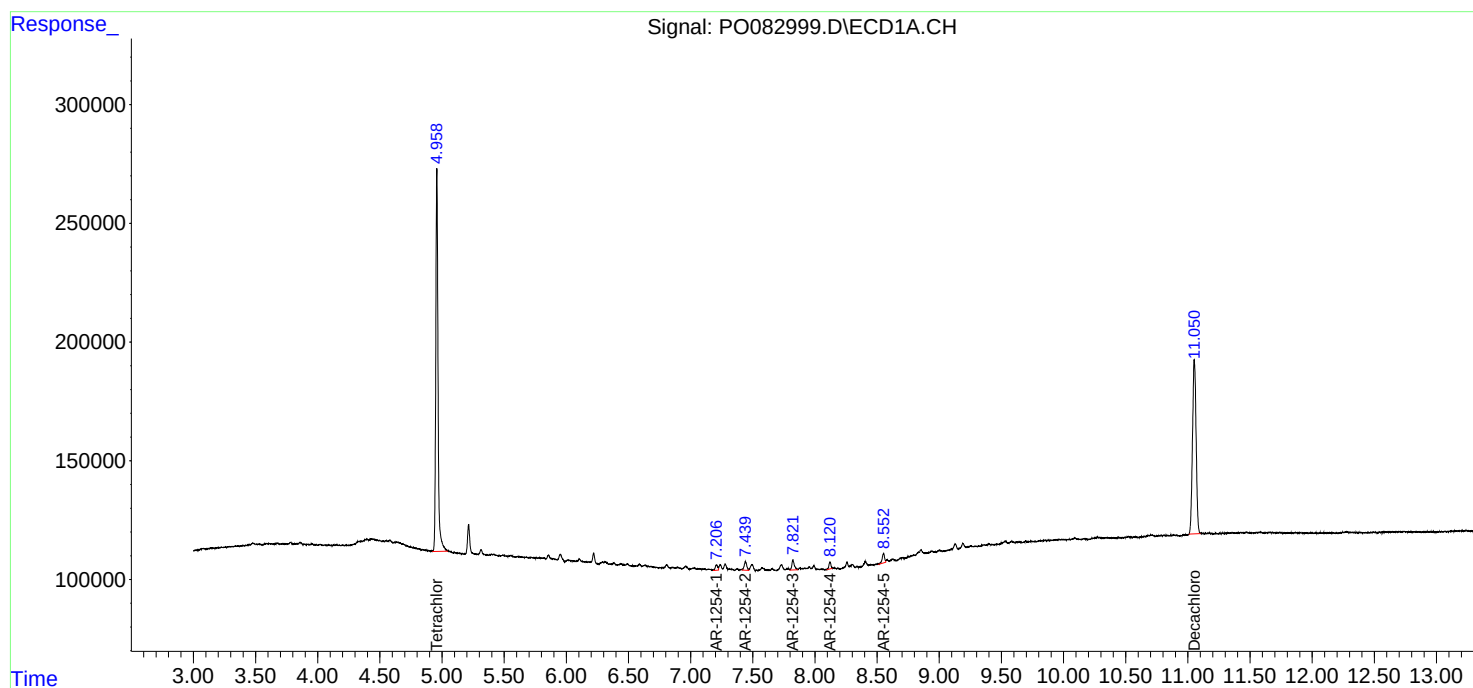

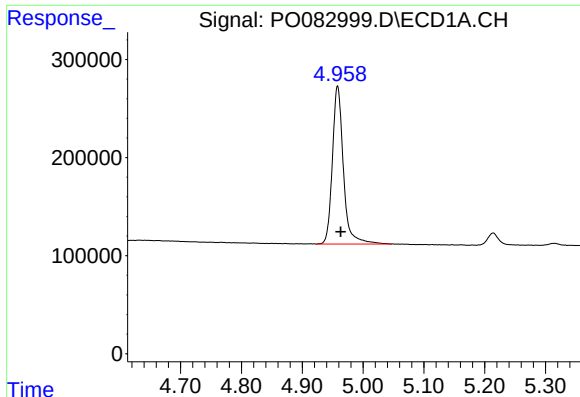


#1 Tetrachloro-m-xylene

R.T.: 4.958 min
Delta R.T.: -0.005 min
Response: 2032214
Conc: 22.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
FLOOR-1-ROOM-2-PILLARS


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :mohammad ahmed 11/18/2021

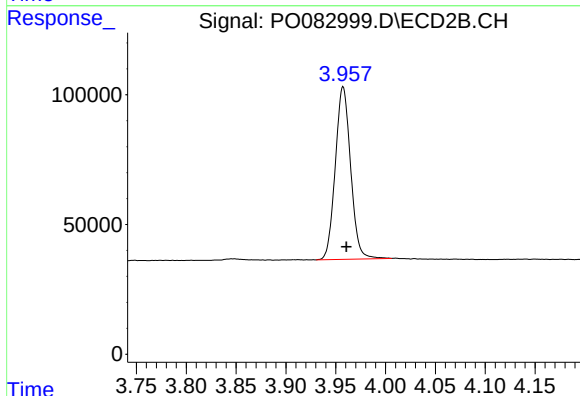


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.003 min
Response: 712002
Conc: 21.94 ng/ml

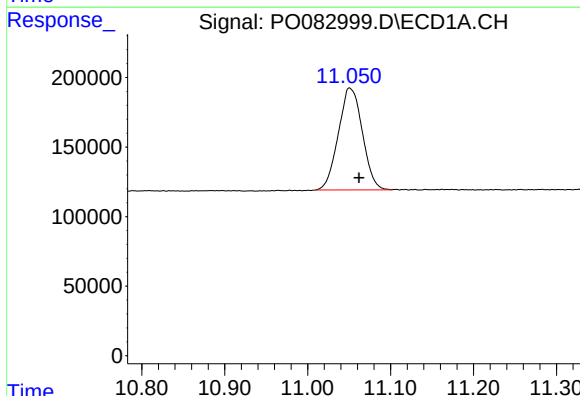


#2 Decachlorobiphenyl

R.T.: 11.050 min
Delta R.T.: -0.012 min
Response: 1475725
Conc: 25.48 ng/ml

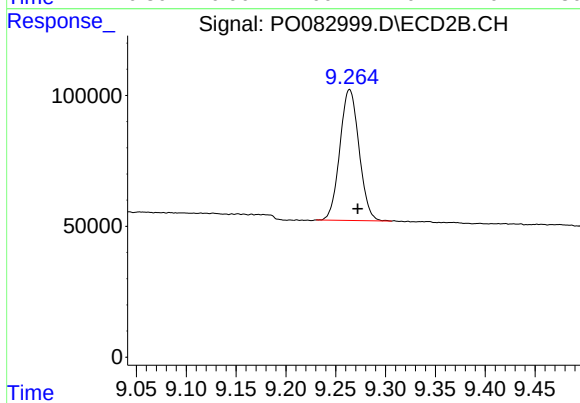

#2 Decachlorobiphenyl

R.T.: 9.264 min
Delta R.T.: -0.008 min
Response: 670135
Conc: 23.64 ng/ml

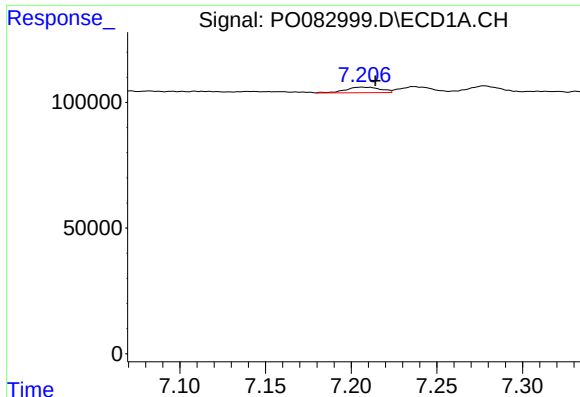


#26 AR-1254-1

R.T.: 7.206 min
Delta R.T.: -0.008 min
Response: 30904
Conc: 11.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
FLOOR-1-ROOM-2-PILLARS


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :mohammad ahmed 11/18/2021

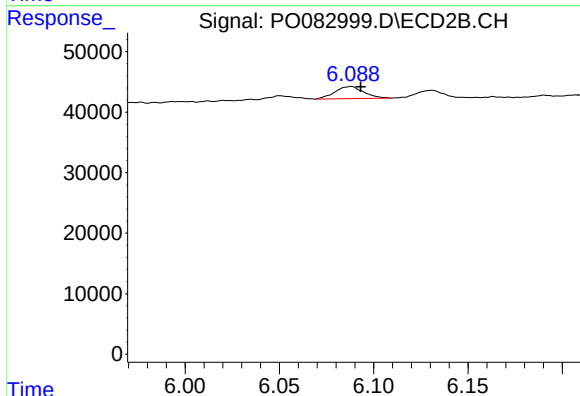


#26 AR-1254-1

R.T.: 6.088 min
Delta R.T.: -0.005 min
Response: 21221
Conc: 10.29 ng/ml

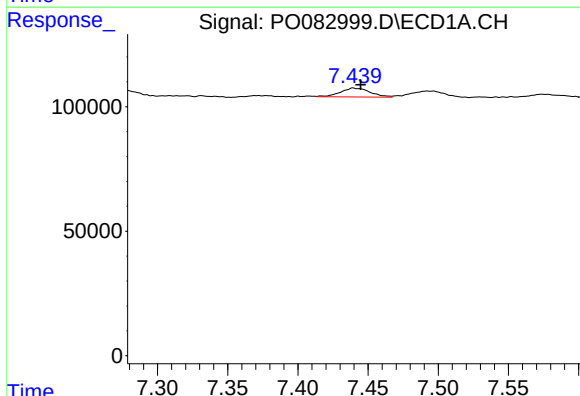


#27 AR-1254-2

R.T.: 7.439 min
Delta R.T.: -0.006 min
Response: 52988
Conc: 12.50 ng/ml

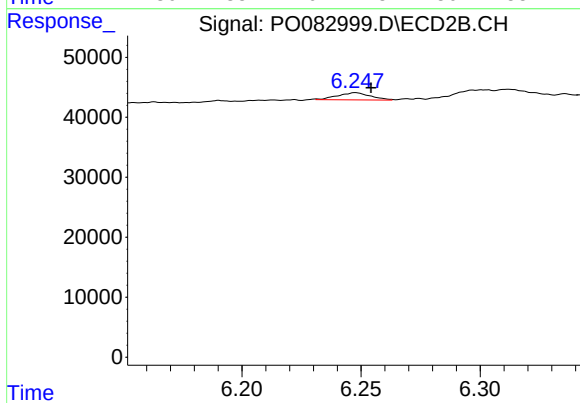

#27 AR-1254-2

R.T.: 6.247 min
Delta R.T.: -0.007 min
Response: 11607
Conc: 6.43 ng/ml m

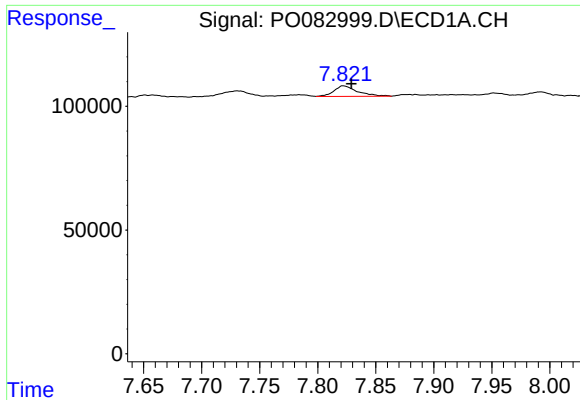


#28 AR-1254-3

R.T.: 7.822 min
Delta R.T.: -0.007 min
Response: 59789
Conc: 14.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
FLOOR-1-ROOM-2-PILLARS


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :mohammad ahmed 11/18/2021

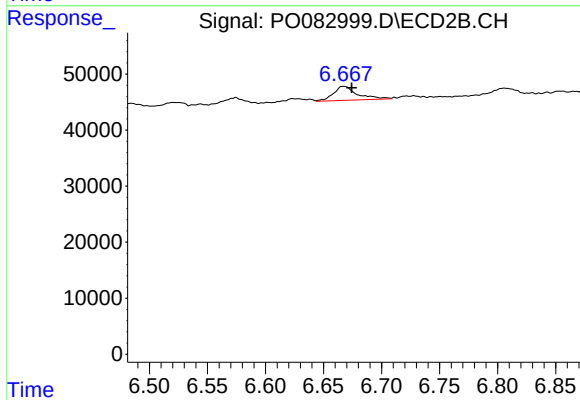


#28 AR-1254-3

R.T.: 6.667 min
Delta R.T.: -0.007 min
Response: 35933
Conc: 12.96 ng/ml

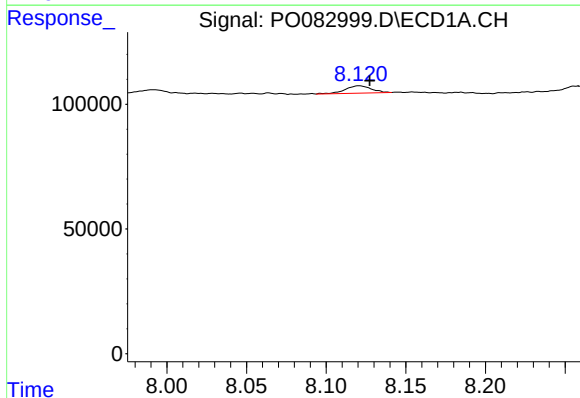


#29 AR-1254-4

R.T.: 8.121 min
Delta R.T.: -0.007 min
Response: 33717
Conc: 11.30 ng/ml

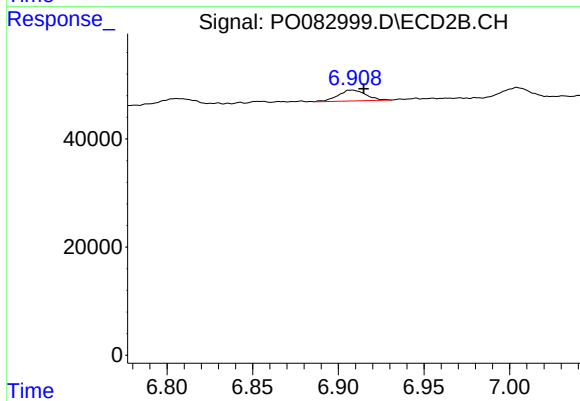

#29 AR-1254-4

R.T.: 6.908 min
Delta R.T.: -0.007 min
Response: 22904
Conc: 11.43 ng/ml

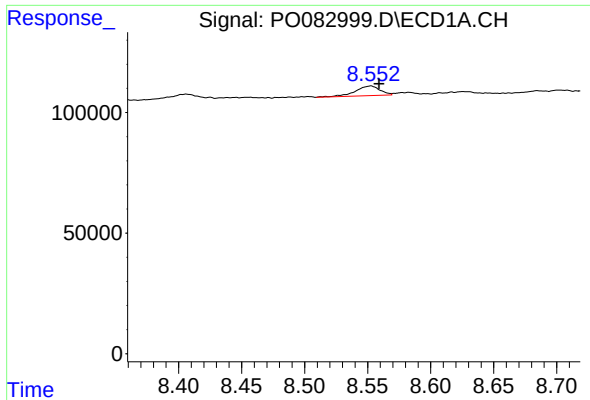


#30 AR-1254-5

R.T.: 8.553 min
Delta R.T.: -0.006 min
Response: 54719
Conc: 17.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
FLOOR-1-ROOM-2-PILLARS

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :mohammad ahmed 11/18/2021

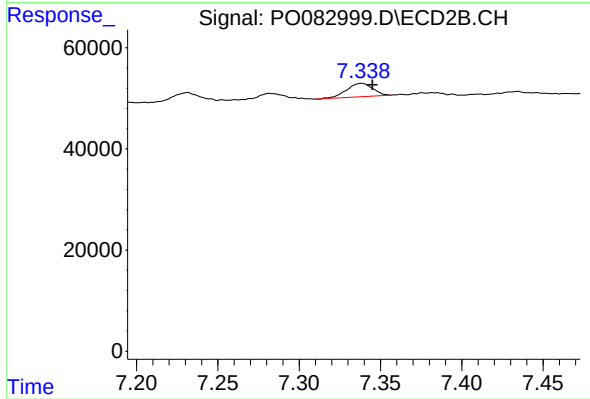

#30 AR-1254-5

R.T.: 7.339 min
Delta R.T.: -0.007 min
Response: 29604
Conc: 11.71 ng/ml