

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111721\
 Data File : PO083003.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Nov 2021 19:34
 Operator : AJ\MA
 Sample : M4724-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 INTERIOR-BRICK-1ST-FLOOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 01:20:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.960	3.959	1864404	678135	20.908	20.899
2) SA Decachlor...	11.054	9.265	1386877	613147	23.947	21.626

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111721\
Data File : PO083003.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2021 19:34
Operator : AJ\MA
Sample : M4724-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
EXTERIOR-BRICK-1ST-FLOOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 01:20:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

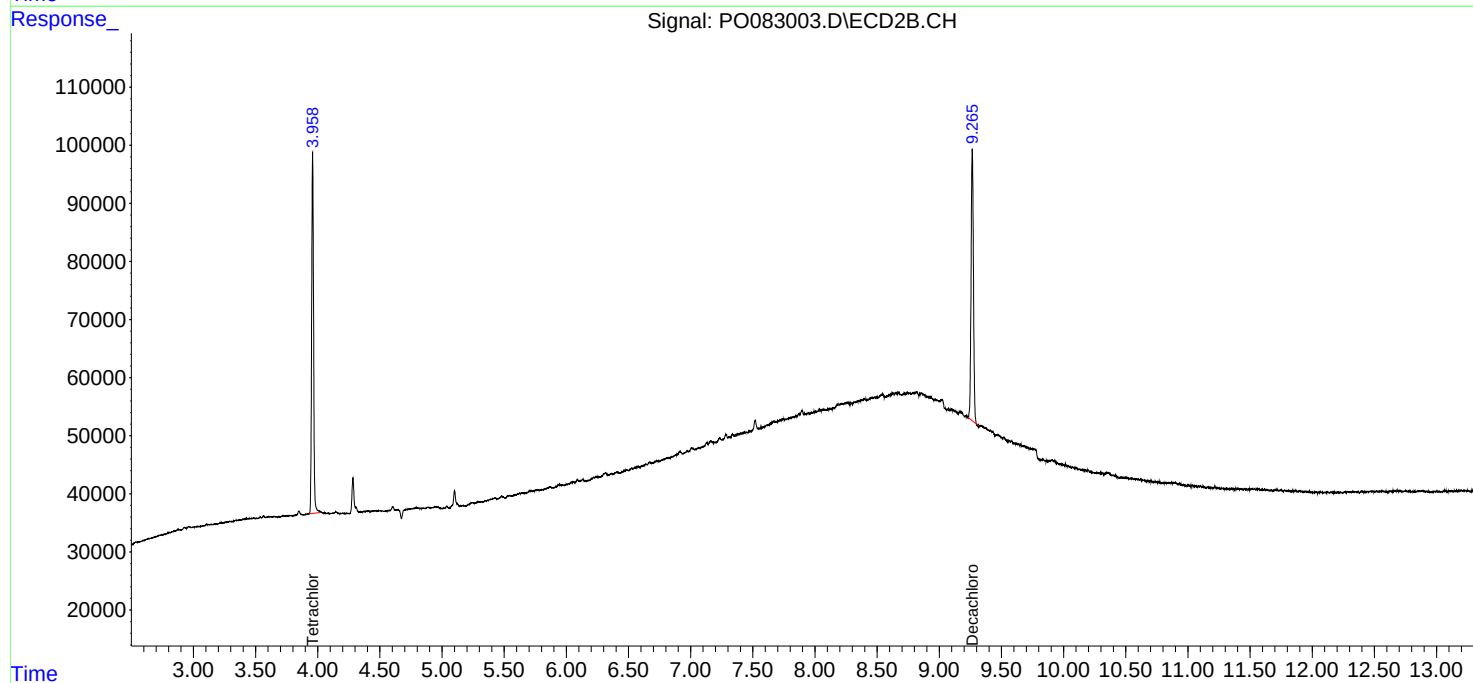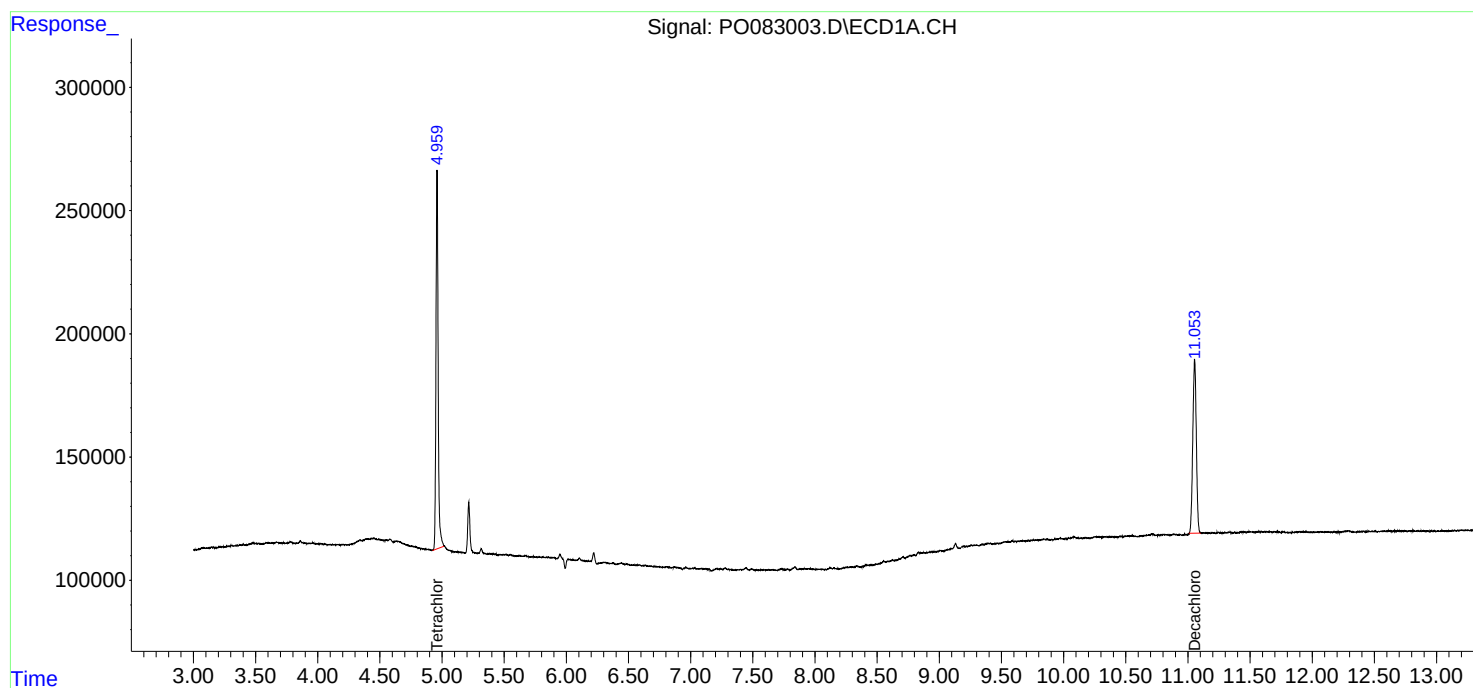


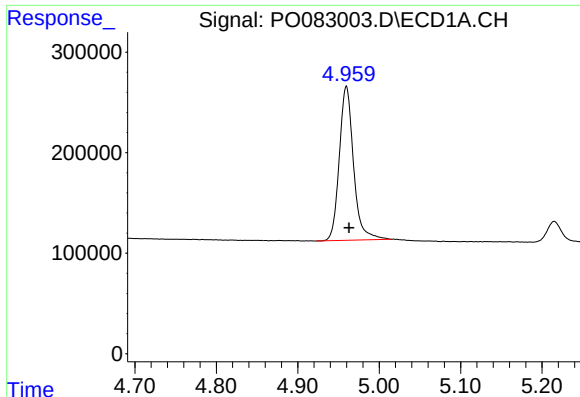

#1 Tetrachloro-m-xylene


R.T.: 4.960 min
Delta R.T.: -0.003 min
Response: 1864404
Conc: 20.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
EXTERIOR-BRICK-1ST-FLOOR

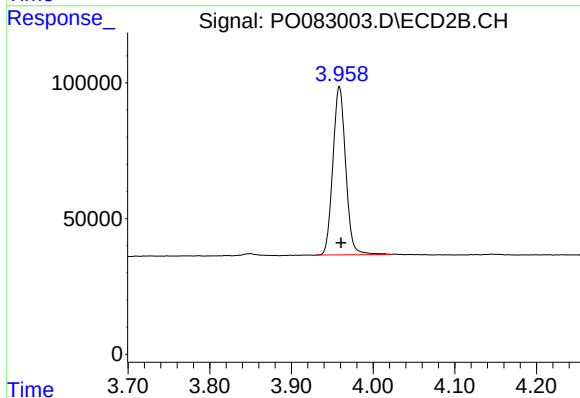


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: -0.002 min
Response: 678135
Conc: 20.90 ng/ml

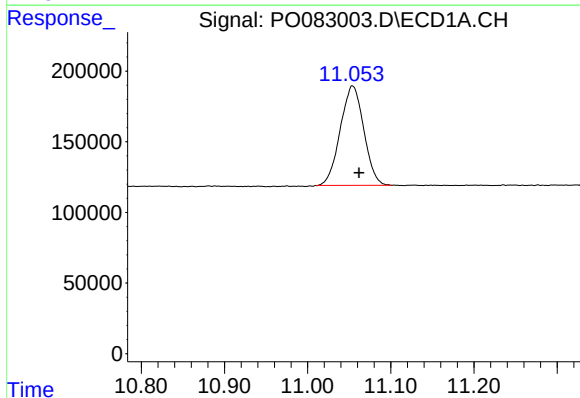

#2 Decachlorobiphenyl

R.T.: 11.054 min
Delta R.T.: -0.008 min
Response: 1386877
Conc: 23.95 ng/ml

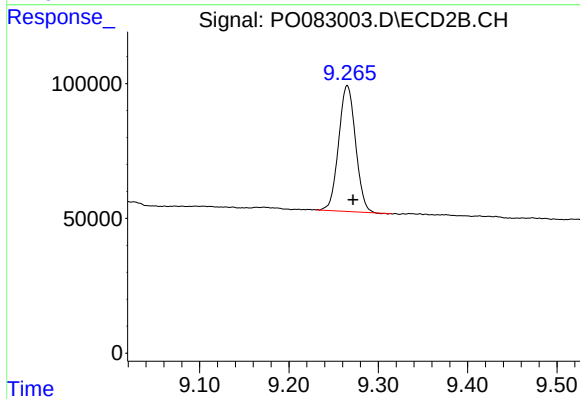

#2 Decachlorobiphenyl

R.T.: 9.265 min
Delta R.T.: -0.007 min
Response: 613147
Conc: 21.63 ng/ml