

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111721\
 Data File : PO083015.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Nov 2021 23:35
 Operator : AJ\MA
 Sample : M4724-13
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 3RD-FLOOR-BRICK

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
 Supervised By :mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 01:24:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.957	3.956	2098184	717398	23.530	22.109
2) SA Decachlor...	11.049	9.263	1503828	667175	25.966m	23.531
Target Compounds						
31) L7 AR-1260-1	7.989	6.804	48293	33063	16.232m	17.157
32) L7 AR-1260-2	8.257	7.003	125721	46485	34.230	18.277 #
33) L7 AR-1260-3	8.614f	7.154	68071	69429	24.498m	31.210m#
34) L7 AR-1260-4	8.852	7.641	153292	40895	48.659	23.485 #
35) L7 AR-1260-5	9.187	7.890	131144	81078	21.171	18.513m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111721\
Data File : P0083015.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2021 23:35
Operator : AJ\MA
Sample : M4724-13
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
3RD-FLOOR-BRICK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :mohammad ahmed 11/18/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 01:24:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

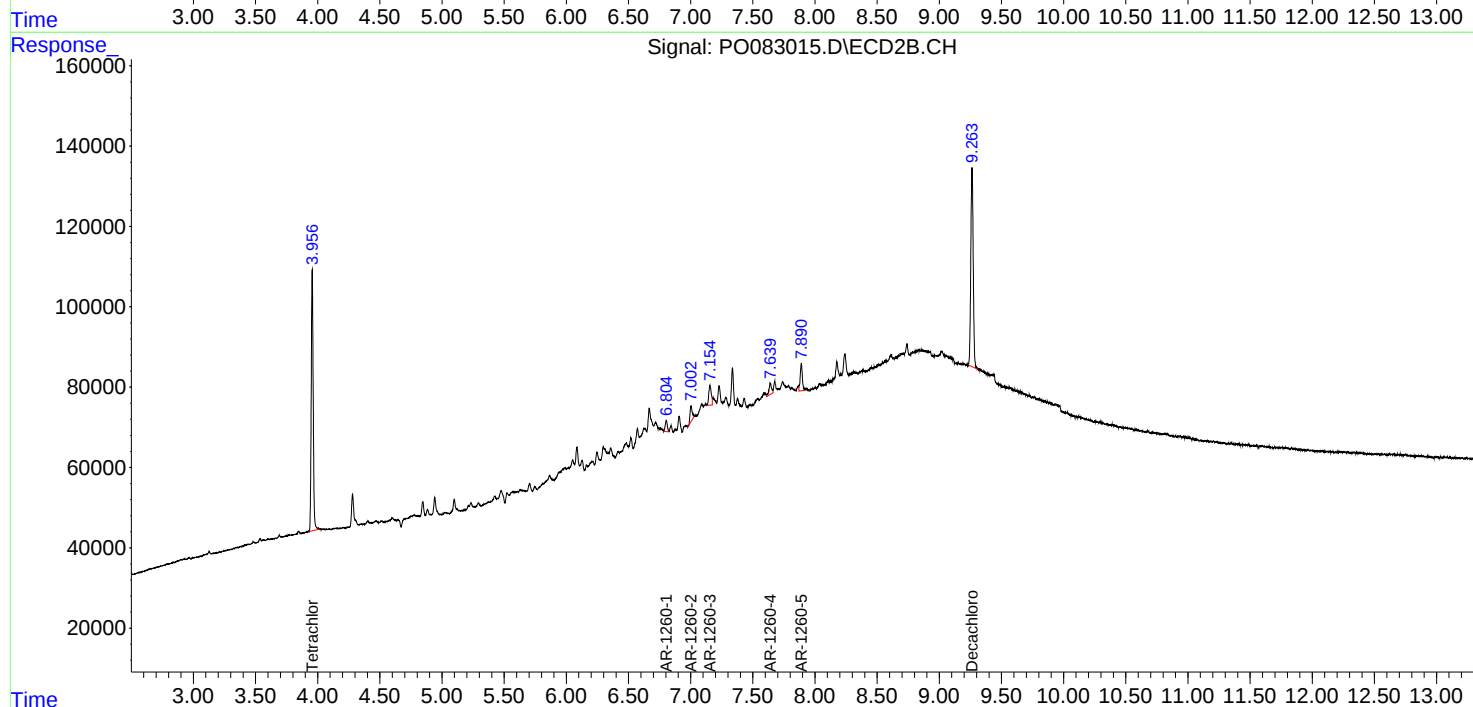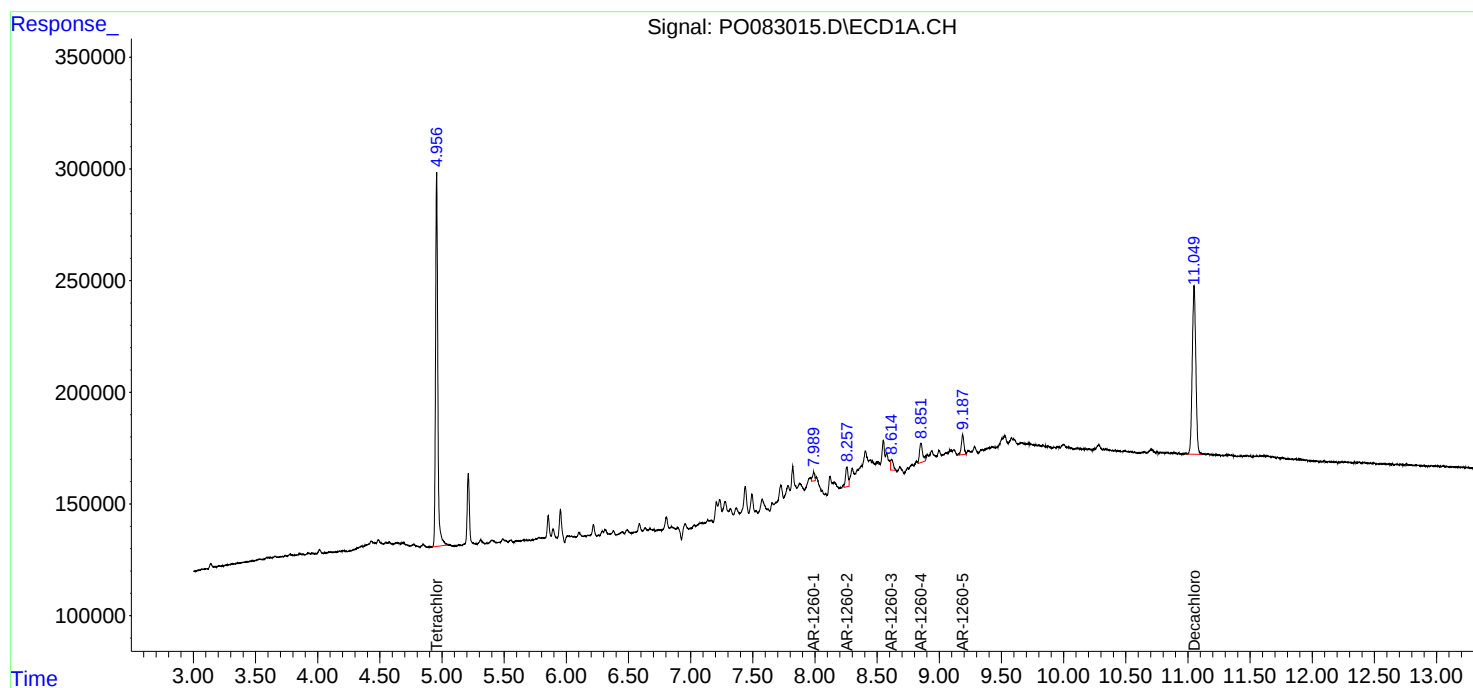

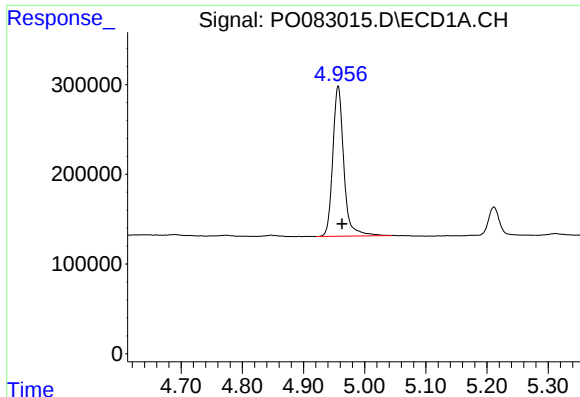


#1 Tetrachloro-m-xylene

R.T.: 4.957 min
Delta R.T.: -0.006 min
Response: 2098184
Conc: 23.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
3RD-FLOOR-BRICK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :mohammad ahmed 11/18/2021

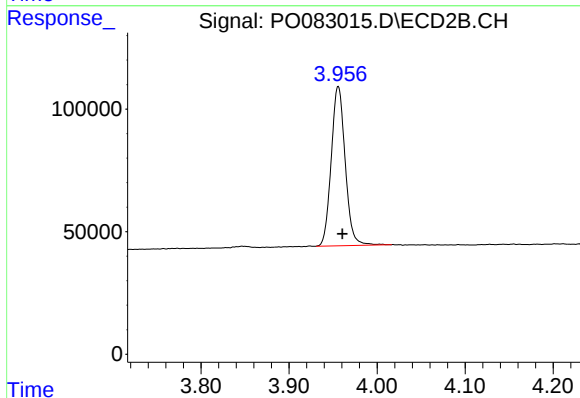


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.005 min
Response: 717398
Conc: 22.11 ng/ml

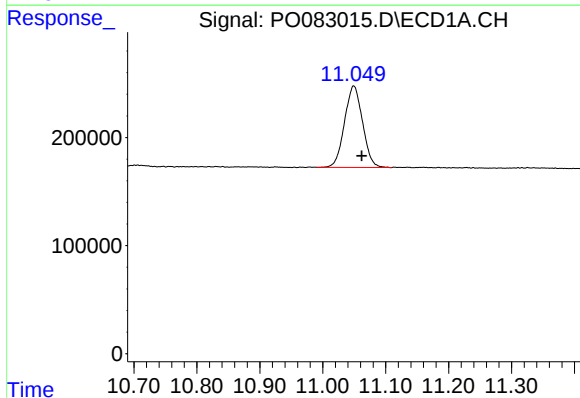


#2 Decachlorobiphenyl

R.T.: 11.049 min
Delta R.T.: -0.013 min
Response: 1503828
Conc: 25.97 ng/ml m

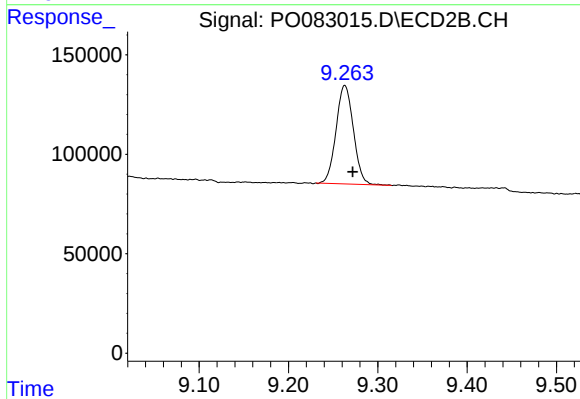

#2 Decachlorobiphenyl

R.T.: 9.263 min
Delta R.T.: -0.009 min
Response: 667175
Conc: 23.53 ng/ml

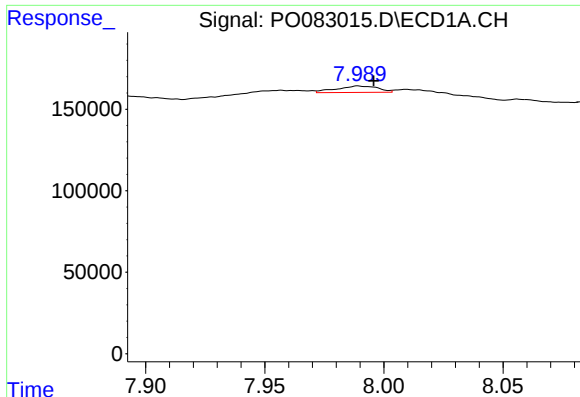


#31 AR-1260-1

R.T.: 7.989 min
Delta R.T.: -0.007 min
Response: 48293
Conc: 16.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
3RD-FLOOR-BRICK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :mohammad ahmed 11/18/2021

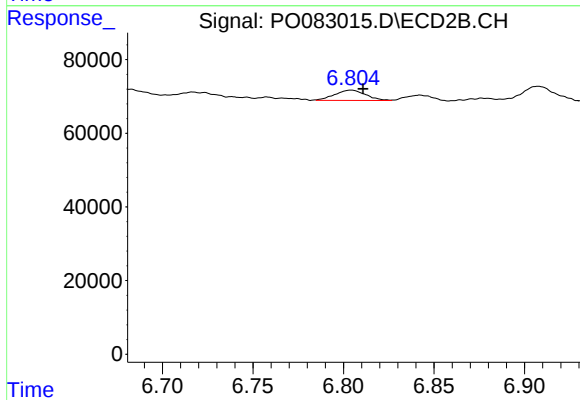


#31 AR-1260-1

R.T.: 6.804 min
Delta R.T.: -0.007 min
Response: 33063
Conc: 17.16 ng/ml

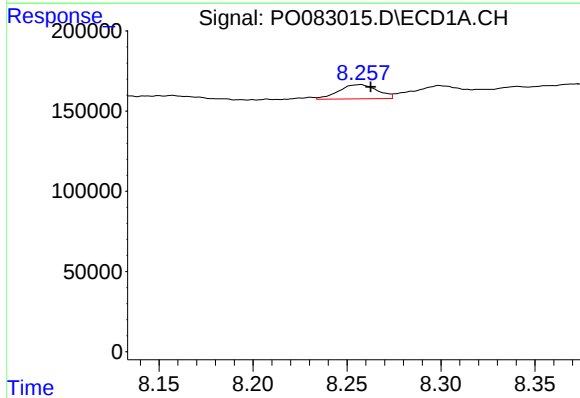


#32 AR-1260-2

R.T.: 8.257 min
Delta R.T.: -0.005 min
Response: 125721
Conc: 34.23 ng/ml

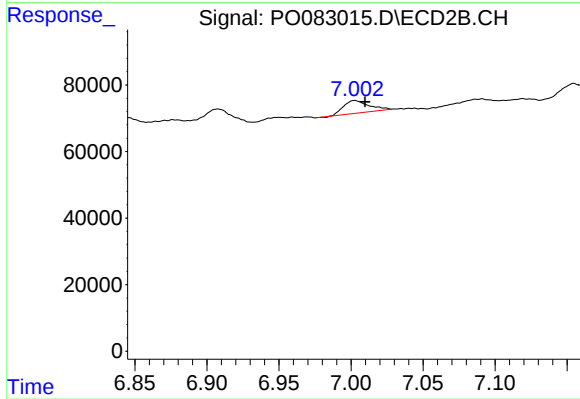

#32 AR-1260-2

R.T.: 7.003 min
Delta R.T.: -0.007 min
Response: 46485
Conc: 18.28 ng/ml

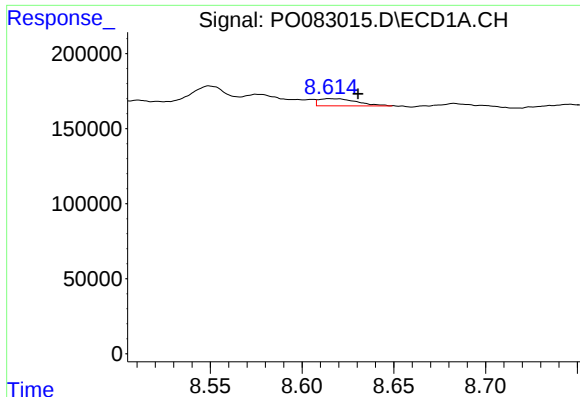


#33 AR-1260-3

R.T.: 8.614 min
Delta R.T.: -0.016 min
Response: 68071
Conc: 24.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
3RD-FLOOR-BRICK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :mohammad ahmed 11/18/2021

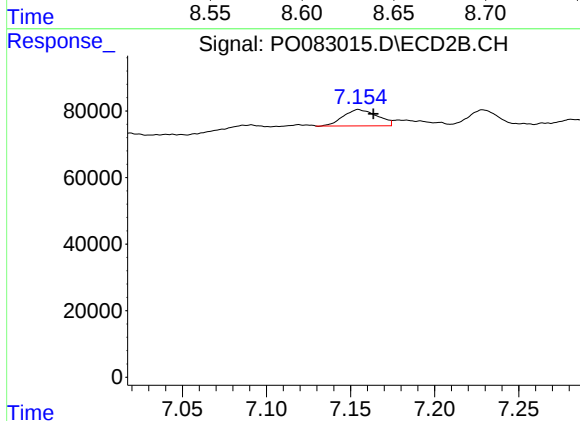


#33 AR-1260-3

R.T.: 7.154 min
Delta R.T.: -0.009 min
Response: 69429
Conc: 31.21 ng/ml m

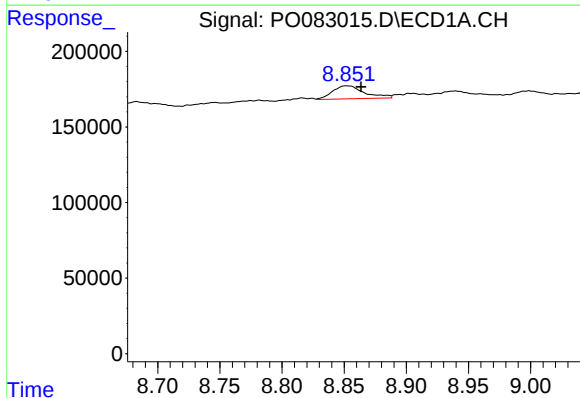


#34 AR-1260-4

R.T.: 8.852 min
Delta R.T.: -0.012 min
Response: 153292
Conc: 48.66 ng/ml

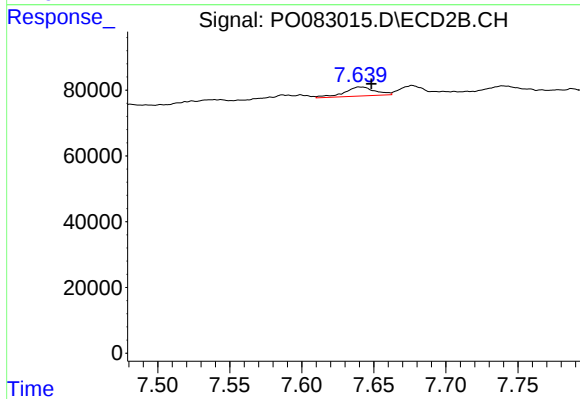

#34 AR-1260-4

R.T.: 7.641 min
Delta R.T.: -0.008 min
Response: 40895
Conc: 23.49 ng/ml

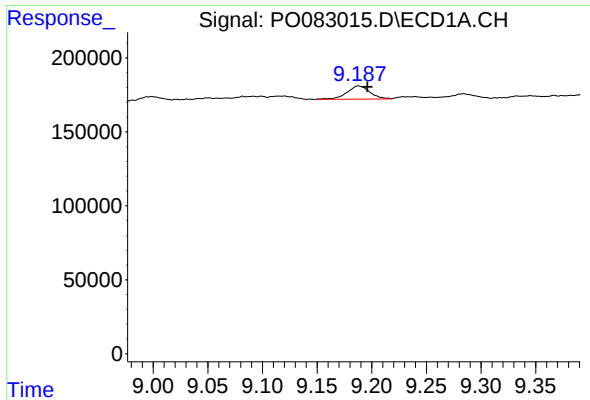


#35 AR-1260-5

R.T.: 9.187 min
Delta R.T.: -0.009 min
Response: 131144
Conc: 21.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
3RD-FLOOR-BRICK

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :mohammad ahmed 11/18/2021

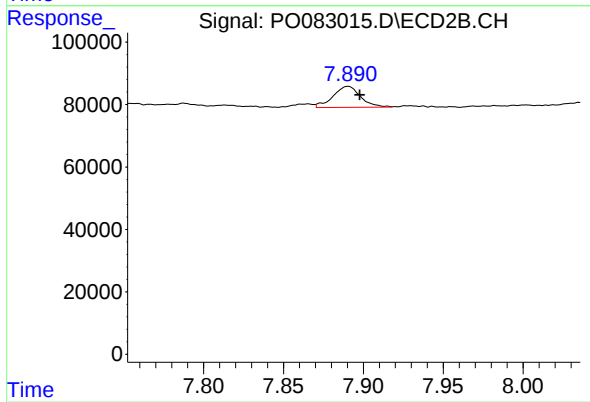

#35 AR-1260-5

R.T.: 7.890 min
Delta R.T.: -0.008 min
Response: 81078
Conc: 18.51 ng/ml m