

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111721\
 Data File : PO083039.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2021 7:38
 Operator : AJ\MA
 Sample : M4705-06 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SEC-2021-44A

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
 Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 11:36:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.955	3.954	146726	55599	1.645m	1.713m
2) SA Decachlor...	11.049	9.262	139281	44697	2.405	1.576 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111721\
Data File : PO083039.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2021 7:38
Operator : AJ\MA
Sample : M4705-06 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SEC-2021-44A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 11:36:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

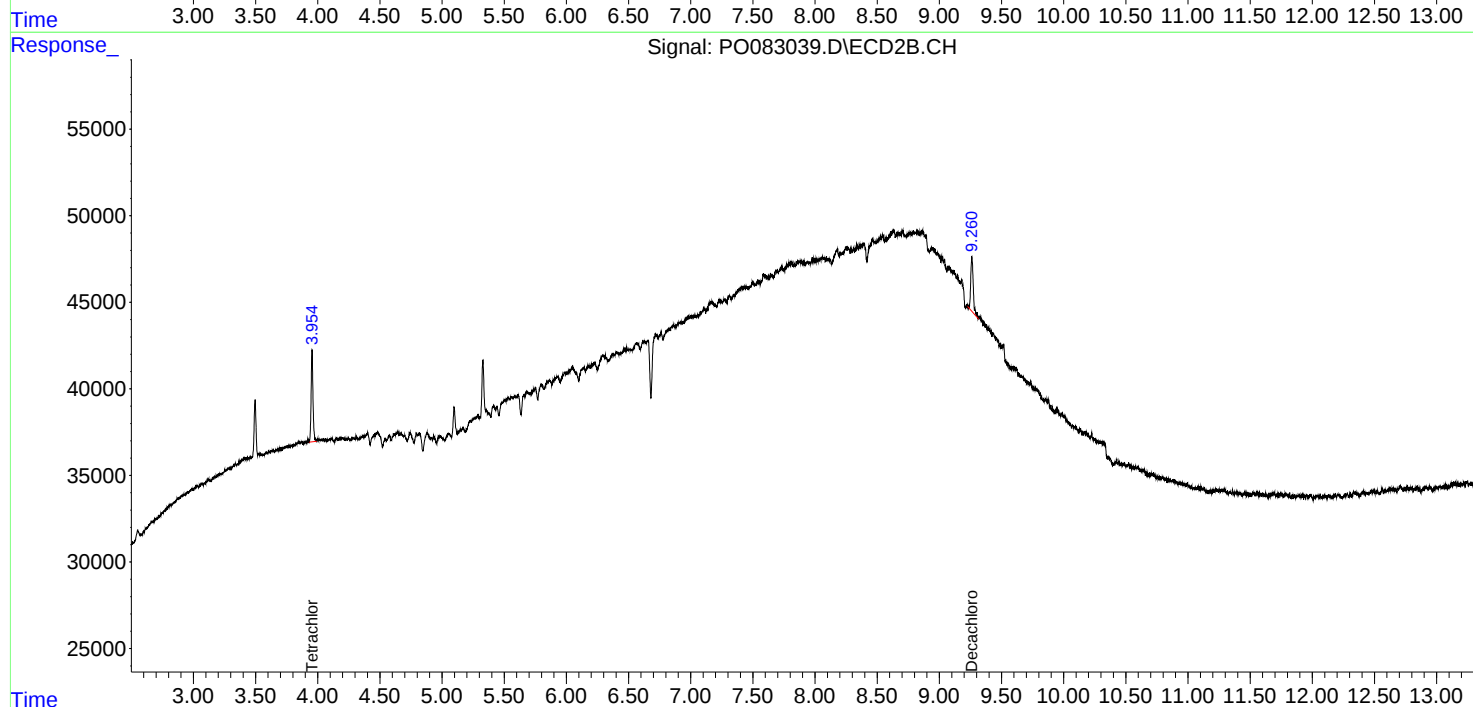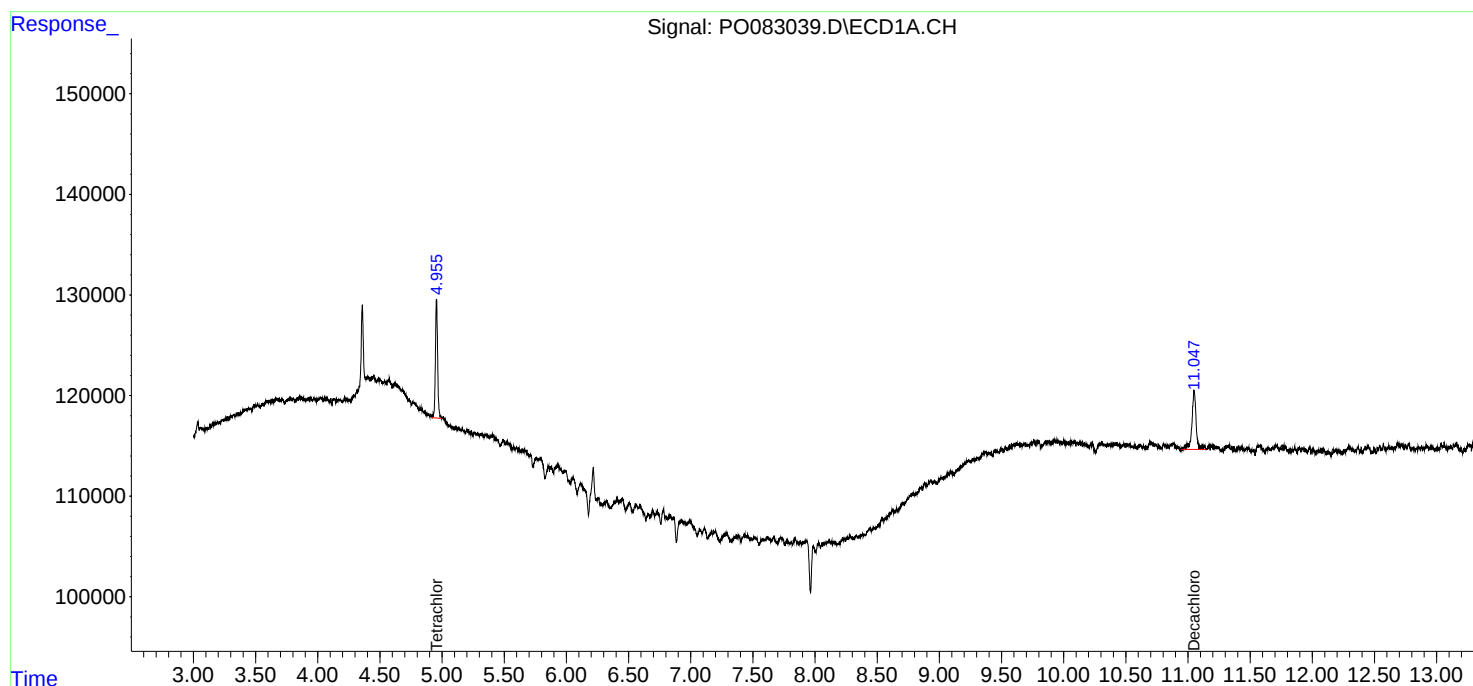

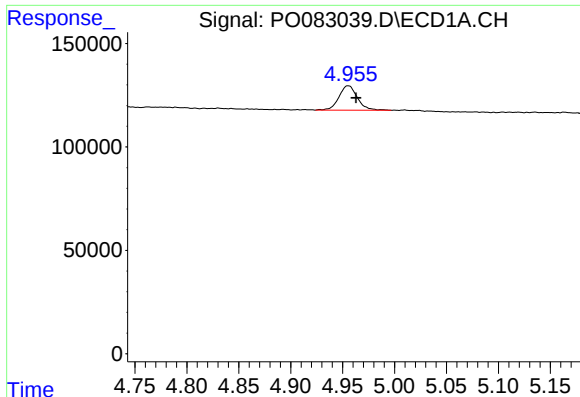


#1 Tetrachloro-m-xylene

R.T.: 4.955 min
Delta R.T.: -0.008 min
Response: 146726
Conc: 1.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-44A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :Sohil Jodhani 11/22/2021

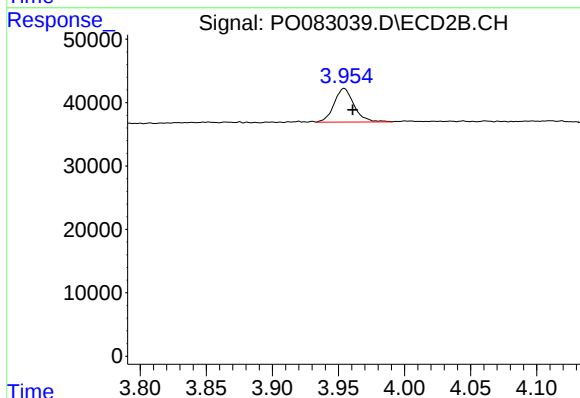


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.007 min
Response: 55599
Conc: 1.71 ng/ml m

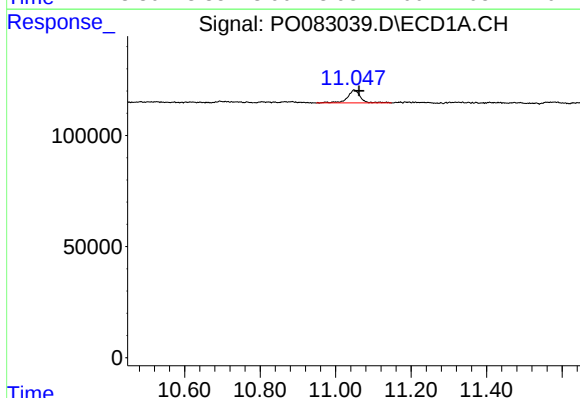

#2 Decachlorobiphenyl

R.T.: 11.049 min
Delta R.T.: -0.013 min
Response: 139281
Conc: 2.40 ng/ml

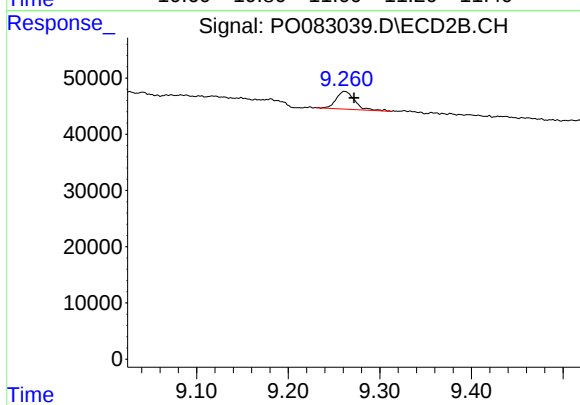

#2 Decachlorobiphenyl

R.T.: 9.262 min
Delta R.T.: -0.010 min
Response: 44697
Conc: 1.58 ng/ml