

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111721\
 Data File : PO083041.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2021 8:13
 Operator : AJ\MA
 Sample : M4705-09 10X
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SEC-2021-46A

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
 Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 11:36:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.956	3.955	144617	52866	1.622	1.629
2) SA Decachlor...	11.050	9.264	124634	37094	2.152m	1.308m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO111721\
Data File : P0083041.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2021 8:13
Operator : AJ\MA
Sample : M4705-09 10X
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SEC-2021-46A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 11:36:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

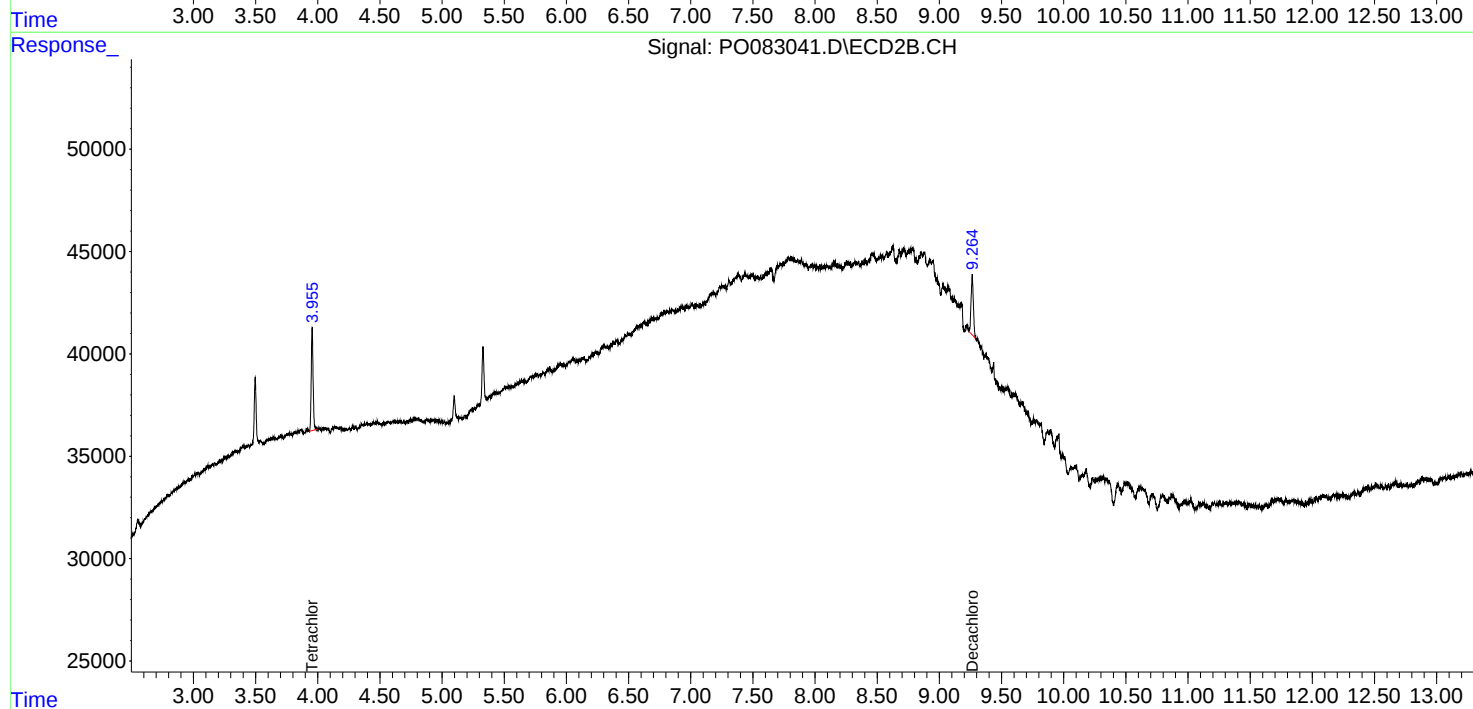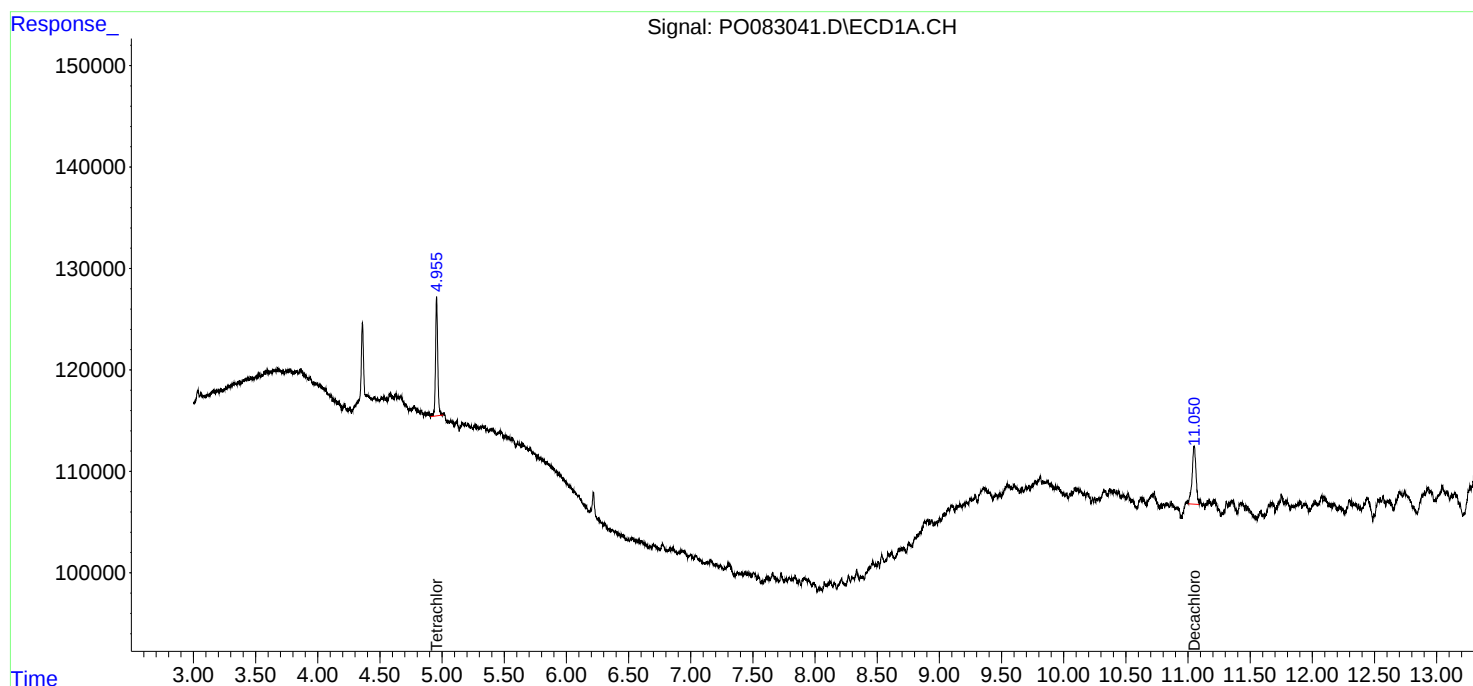

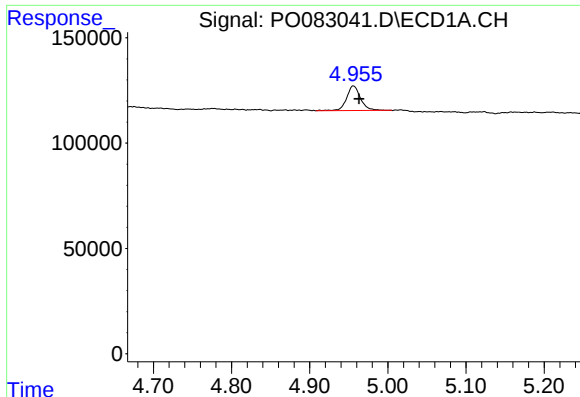


#1 Tetrachloro-m-xylene

R.T.: 4.956 min
Delta R.T.: -0.007 min
Response: 144617
Conc: 1.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
SEC-2021-46A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/18/2021
Supervised By :Sohil Jodhani 11/22/2021

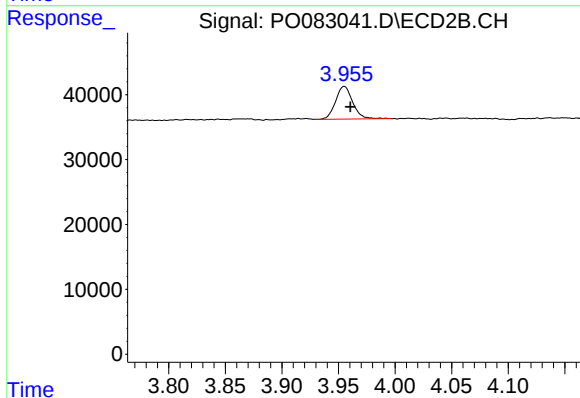


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.005 min
Response: 52866
Conc: 1.63 ng/ml

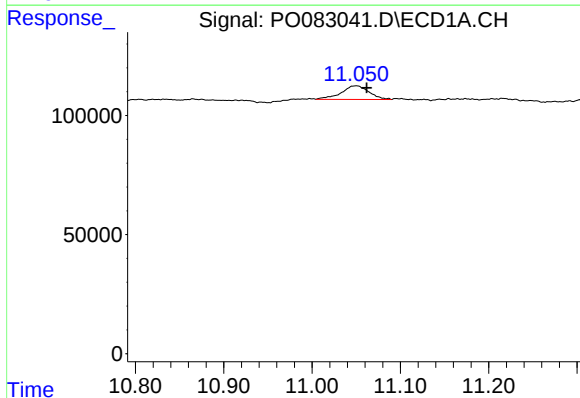

#2 Decachlorobiphenyl

R.T.: 11.050 min
Delta R.T.: -0.012 min
Response: 124634
Conc: 2.15 ng/ml m

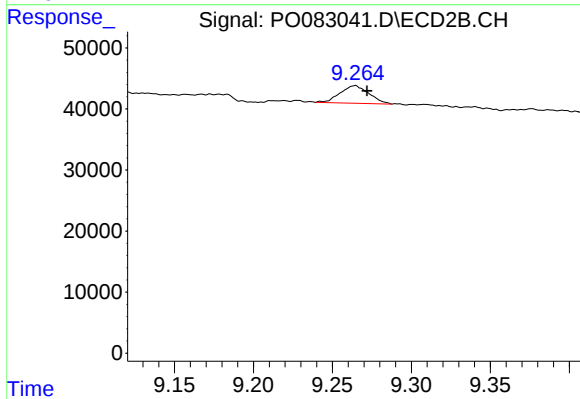

#2 Decachlorobiphenyl

R.T.: 9.264 min
Delta R.T.: -0.008 min
Response: 37094
Conc: 1.31 ng/ml m