

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111723\
 Data File : P0099928.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2023 16:32
 Operator : YP/AJ
 Sample : 05467-03 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KZZ372H-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :Ankita Jodhani 11/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 21:44:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 14 04:21:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.489	3.715	2565491	2025724	1.500m	1.715
2) SA Decachlor...	10.375	8.814	2251040	1894757	2.411	1.930m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111723\
Data File : PO099928.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2023 16:32
Operator : YP/AJ
Sample : 05467-03 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KZZ372H-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :Ankita Jodhani 11/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 21:44:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 14 04:21:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

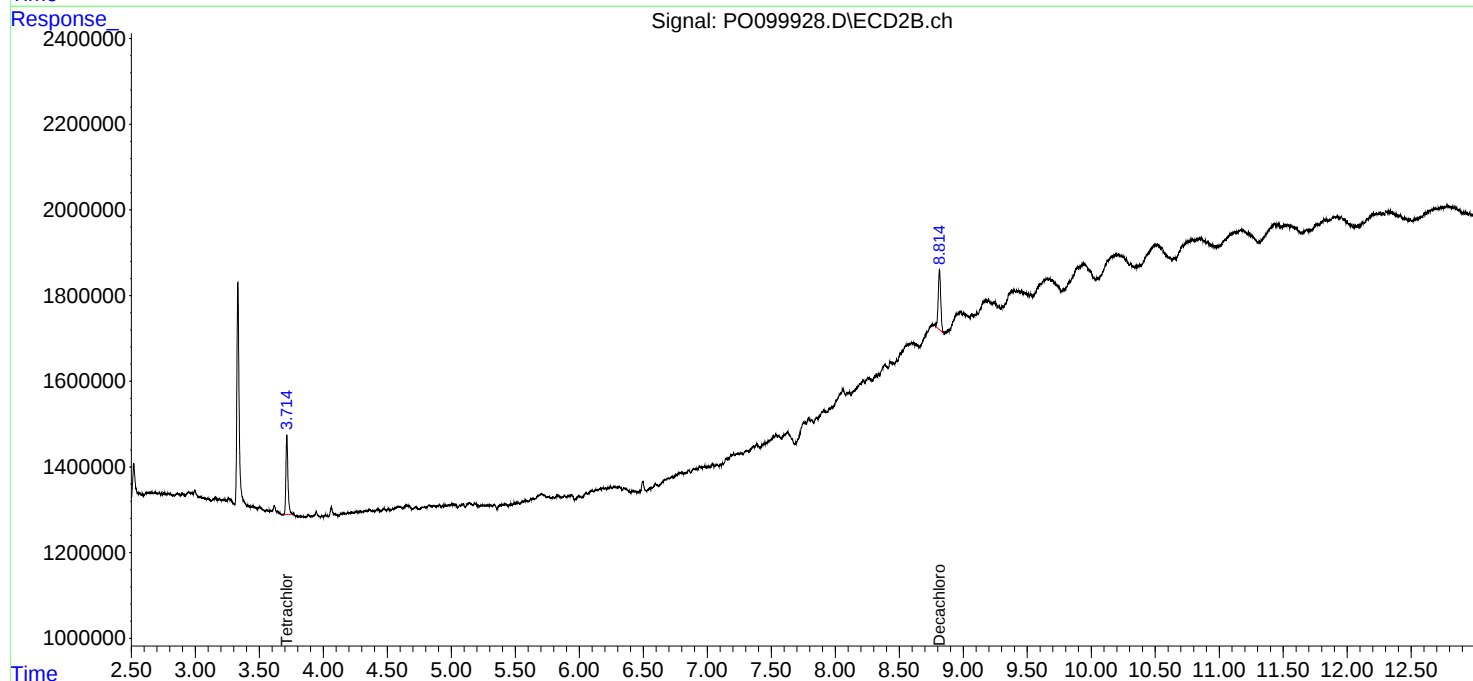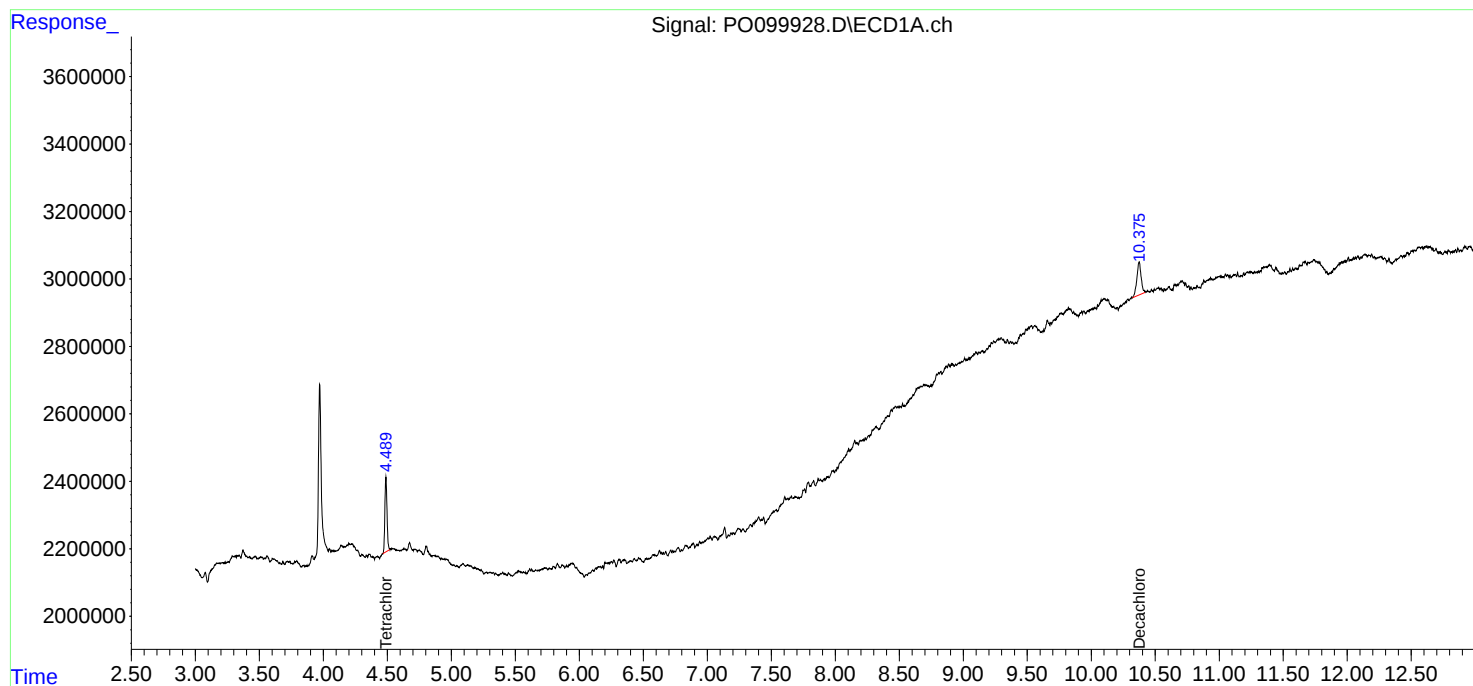

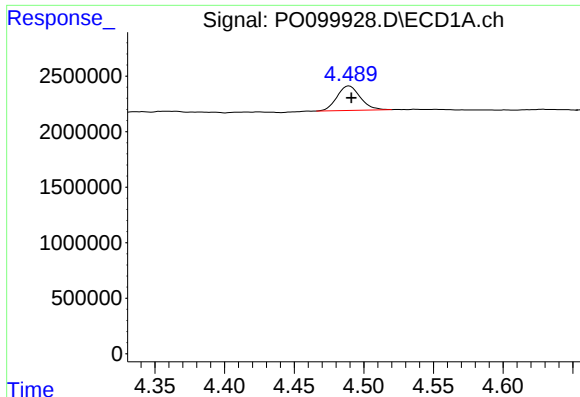


#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: -0.002 min
Response: 2565491
Conc: 1.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
KZZ372H-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :Ankita Jodhani 11/20/2023

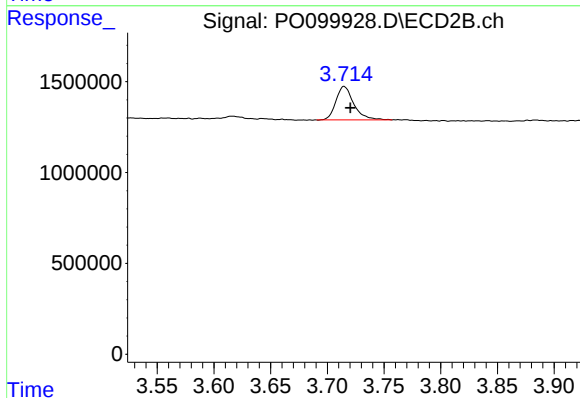


#1 Tetrachloro-m-xylene

R.T.: 3.715 min
Delta R.T.: -0.006 min
Response: 2025724
Conc: 1.71 ng/ml

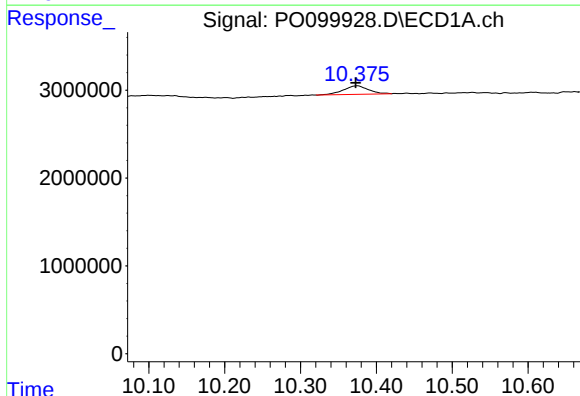

#2 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: 0.002 min
Response: 2251040
Conc: 2.41 ng/ml

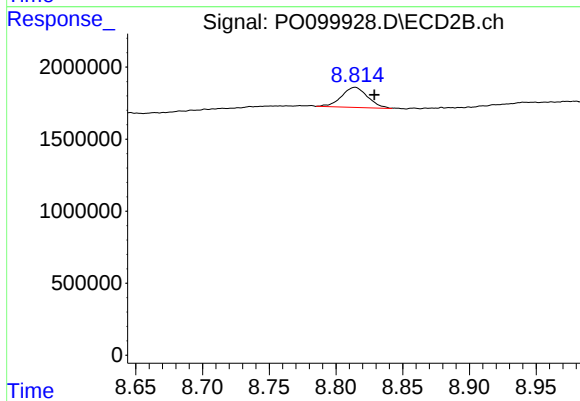

#2 Decachlorobiphenyl

R.T.: 8.814 min
Delta R.T.: -0.015 min
Response: 1894757
Conc: 1.93 ng/ml m