

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111725\
 Data File : P0115137.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2025 13:56
 Operator : YP/AJ
 Sample : Q3639-10 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 L70B

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/19/2025
 Supervised By :Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 10:09:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.347	3.647	7509346	5395210	1.067	1.208
2) SA Decachlor...	9.928	8.639	7020838	6086880	1.588m	1.559m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111725\
Data File : PO115137.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2025 13:56
Operator : YP/AJ
Sample : Q3639-10 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
L70B


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/19/2025
Supervised By :Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 10:09:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

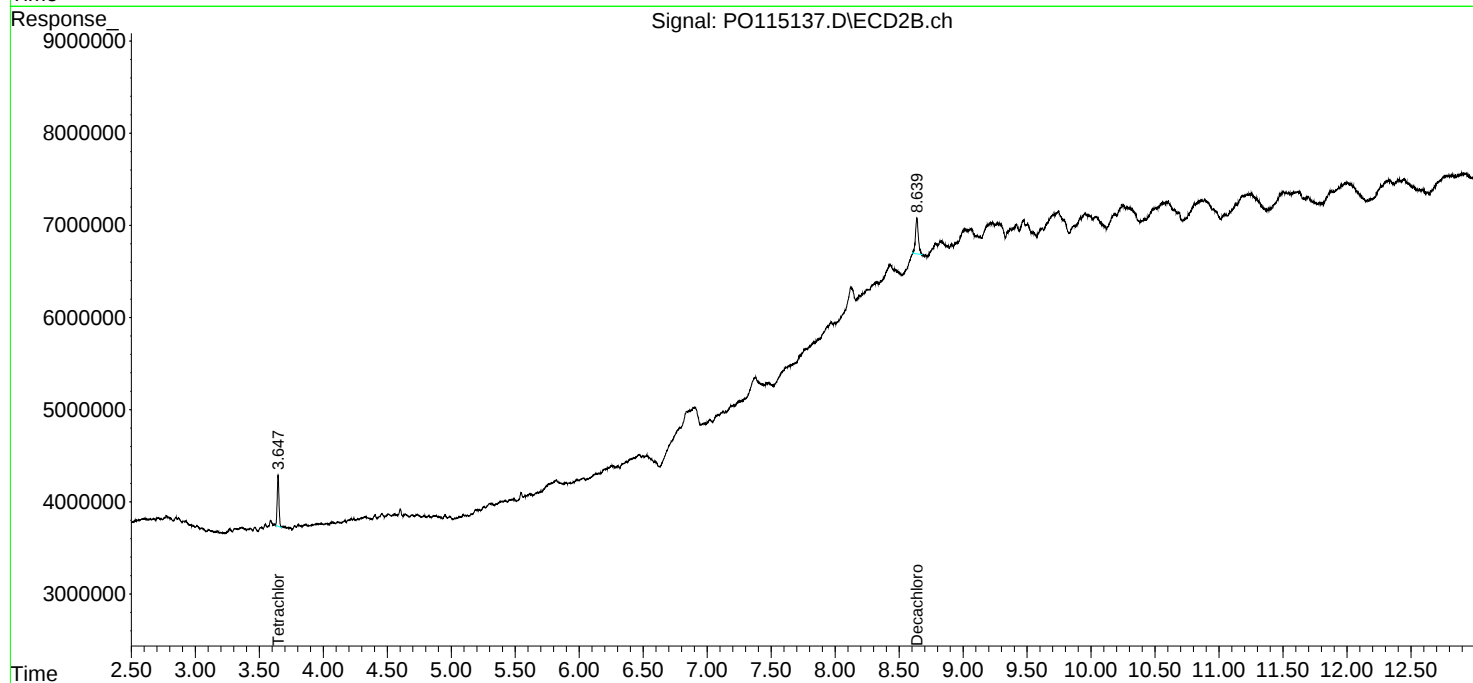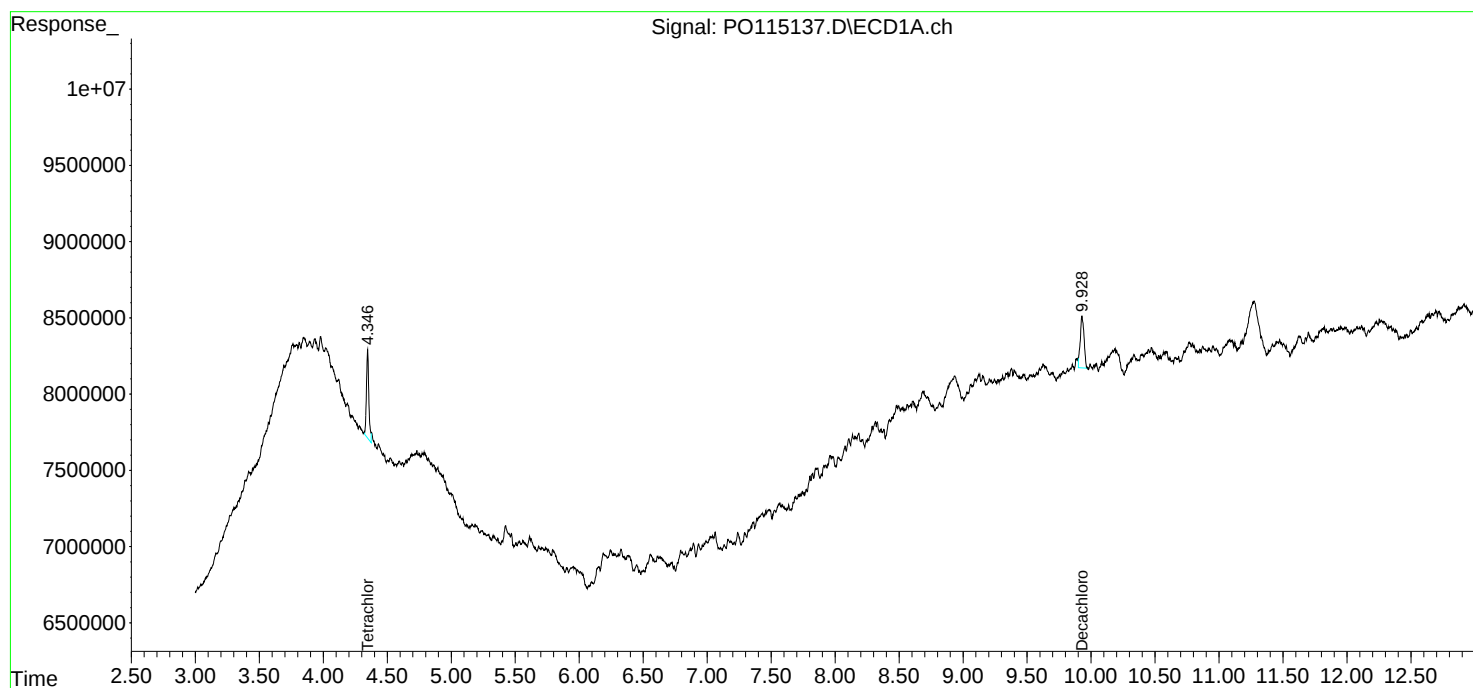

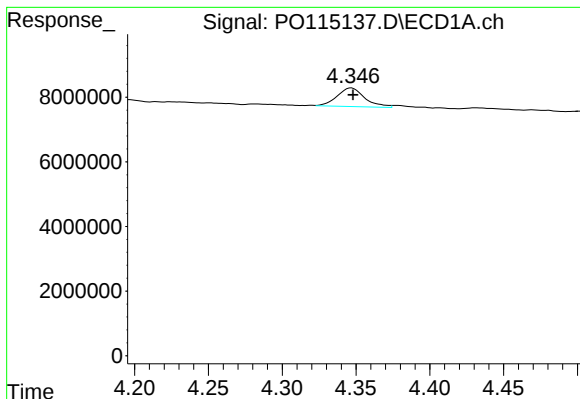


#1 Tetrachloro-m-xylene

R.T.: 4.347 min
Delta R.T.: -0.001 min
Response: 7509346
Conc: 1.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
L70B


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/19/2025
Supervised By :Sohil Jodhani 11/19/2025

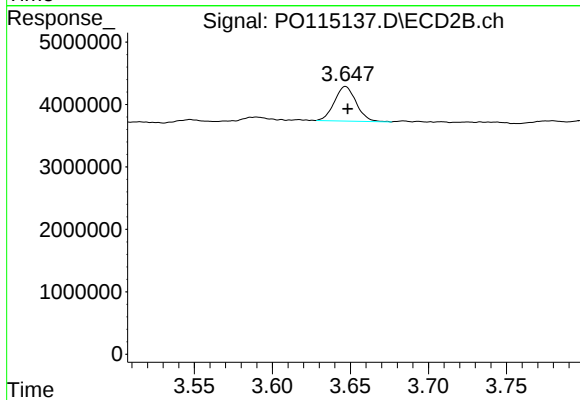


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.001 min
Response: 5395210
Conc: 1.21 ng/ml

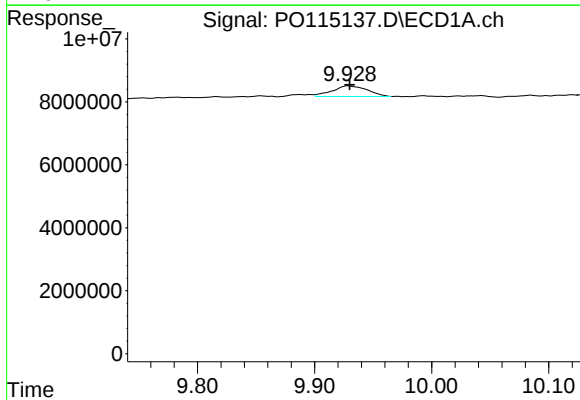

#2 Decachlorobiphenyl

R.T.: 9.928 min
Delta R.T.: -0.002 min
Response: 7020838
Conc: 1.59 ng/ml m

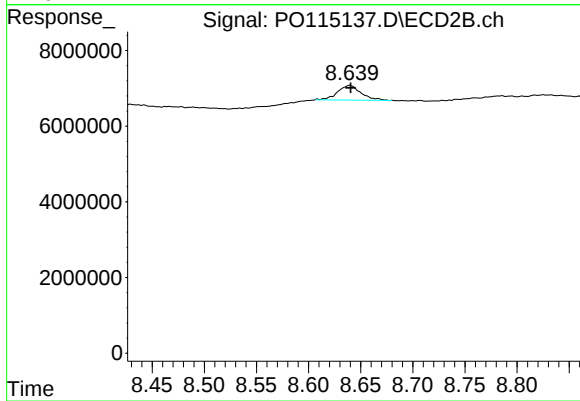

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: -0.002 min
Response: 6086880
Conc: 1.56 ng/ml m