

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111725\
 Data File : P0115163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2025 23:39
 Operator : YP/AJ
 Sample : Q3648-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-02-111425

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/19/2025
 Supervised By :Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 01:44:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.345	3.647	107.3E6	99767640	15.251m	22.335m#
2) SA Decachlor...	9.928	8.636	98794180	71049941	22.350	18.200

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111725\
Data File : PO115163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2025 23:39
Operator : YP/AJ
Sample : Q3648-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-02-111425


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/19/2025
Supervised By :Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 01:44:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

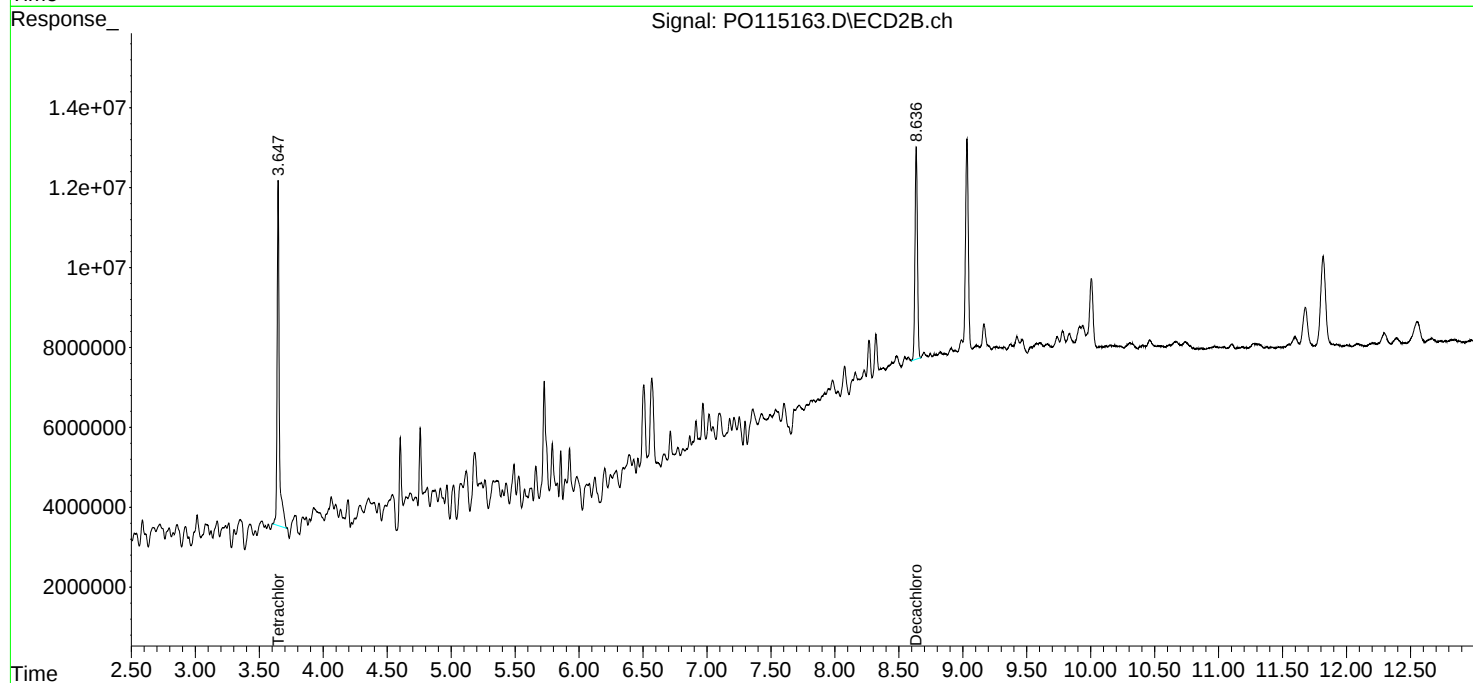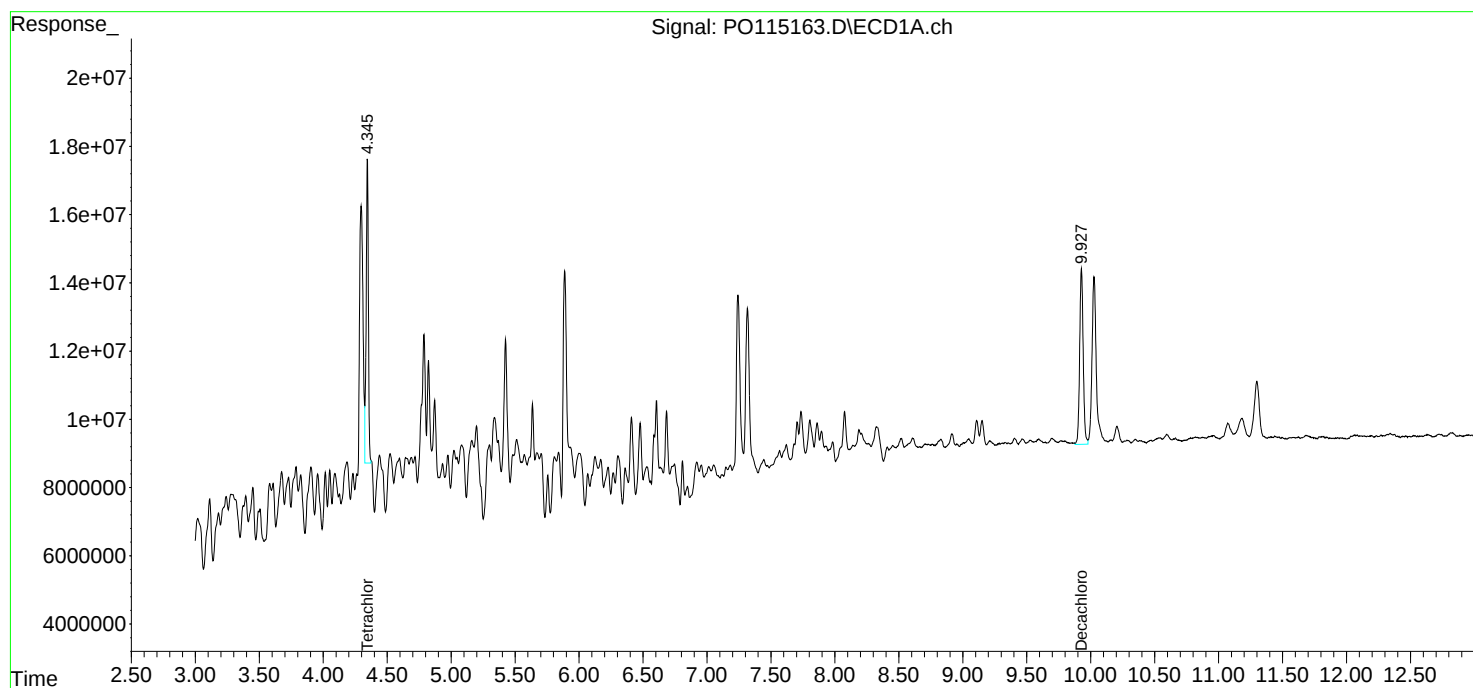

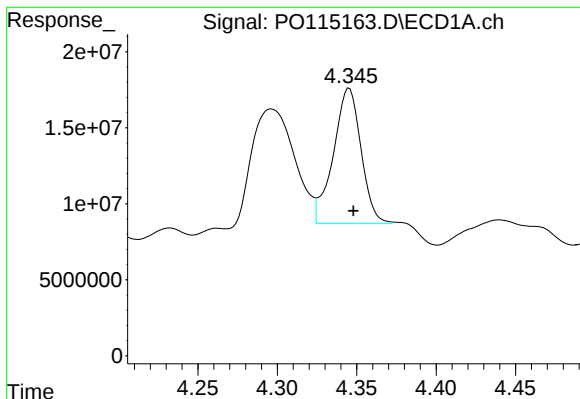

#1 Tetrachloro-m-xylene

R.T.: 4.345 min
Delta R.T.: -0.003 min
Response: 107337640
Conc: 15.25 ng/ml

Instrument :

ECD_O

ClientSampleId :


OR-02-111425

Manual Integrations

APPROVED


Reviewed By :Rahul Chavli 11/19/2025

Supervised By :Sohil Jodhani 11/19/2025

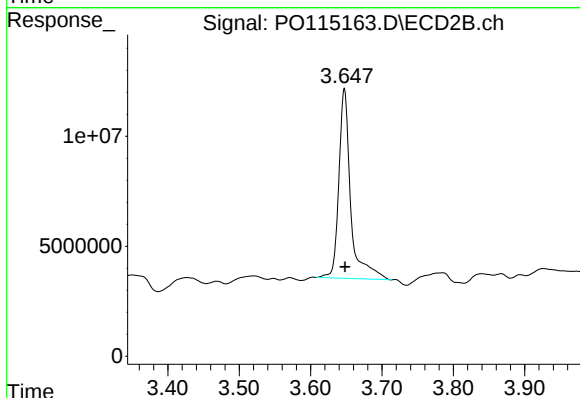


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.001 min
Response: 99767640
Conc: 22.34 ng/ml m

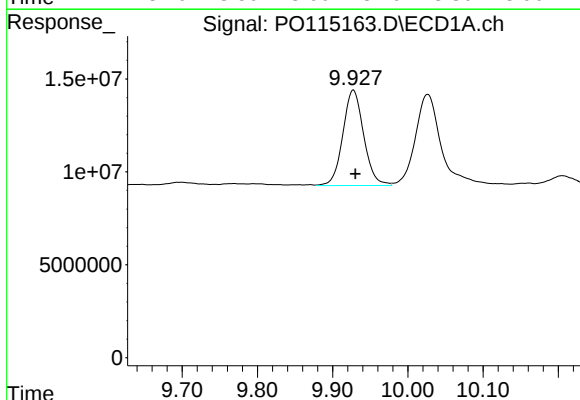

#2 Decachlorobiphenyl

R.T.: 9.928 min
Delta R.T.: -0.002 min
Response: 98794180
Conc: 22.35 ng/ml

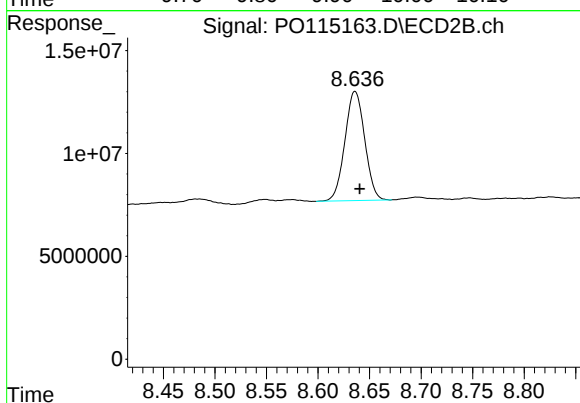

#2 Decachlorobiphenyl

R.T.: 8.636 min
Delta R.T.: -0.005 min
Response: 71049941
Conc: 18.20 ng/ml