

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111725\
 Data File : PO115171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2025 03:37
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:02:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
30) L6 AR-1254-5	7.619	6.713	2087.0E6	2074.8E6	6913.866	5219.349



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO111725\
Data File : PO115171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2025 03:37
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:02:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

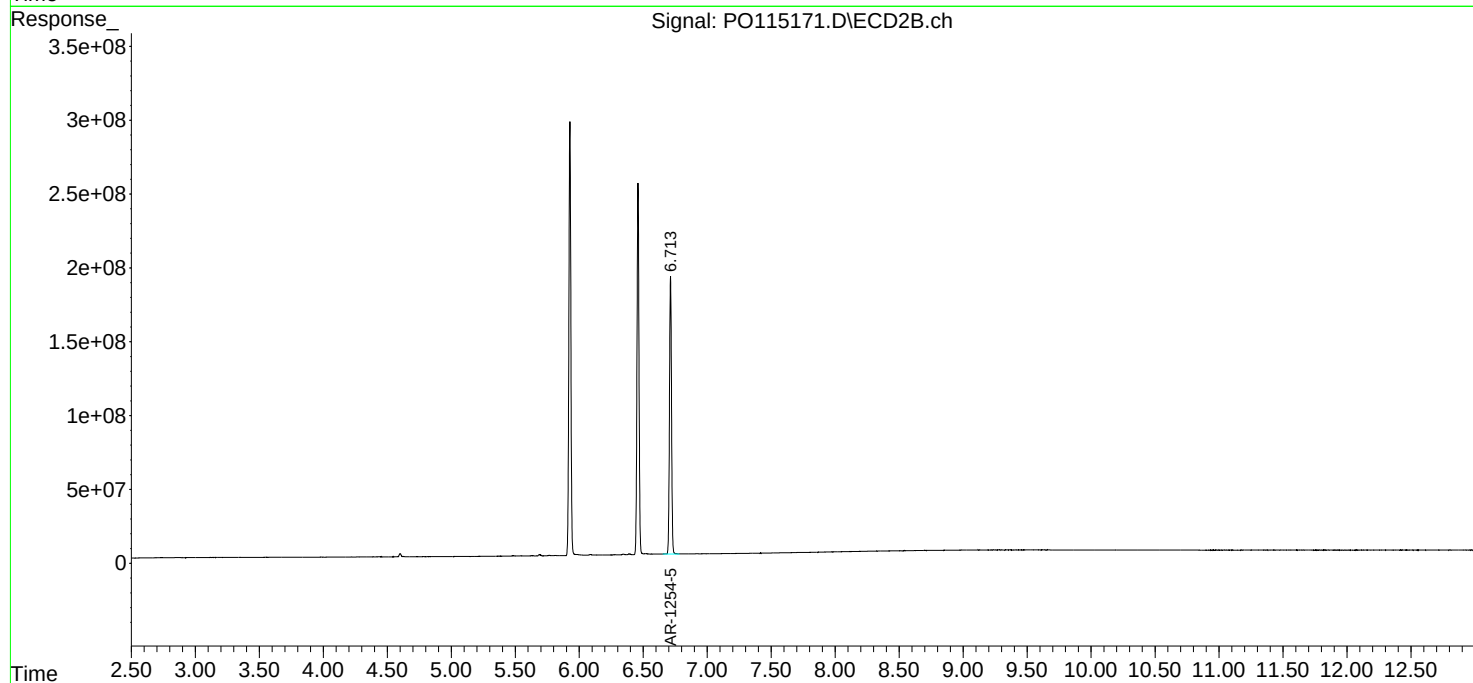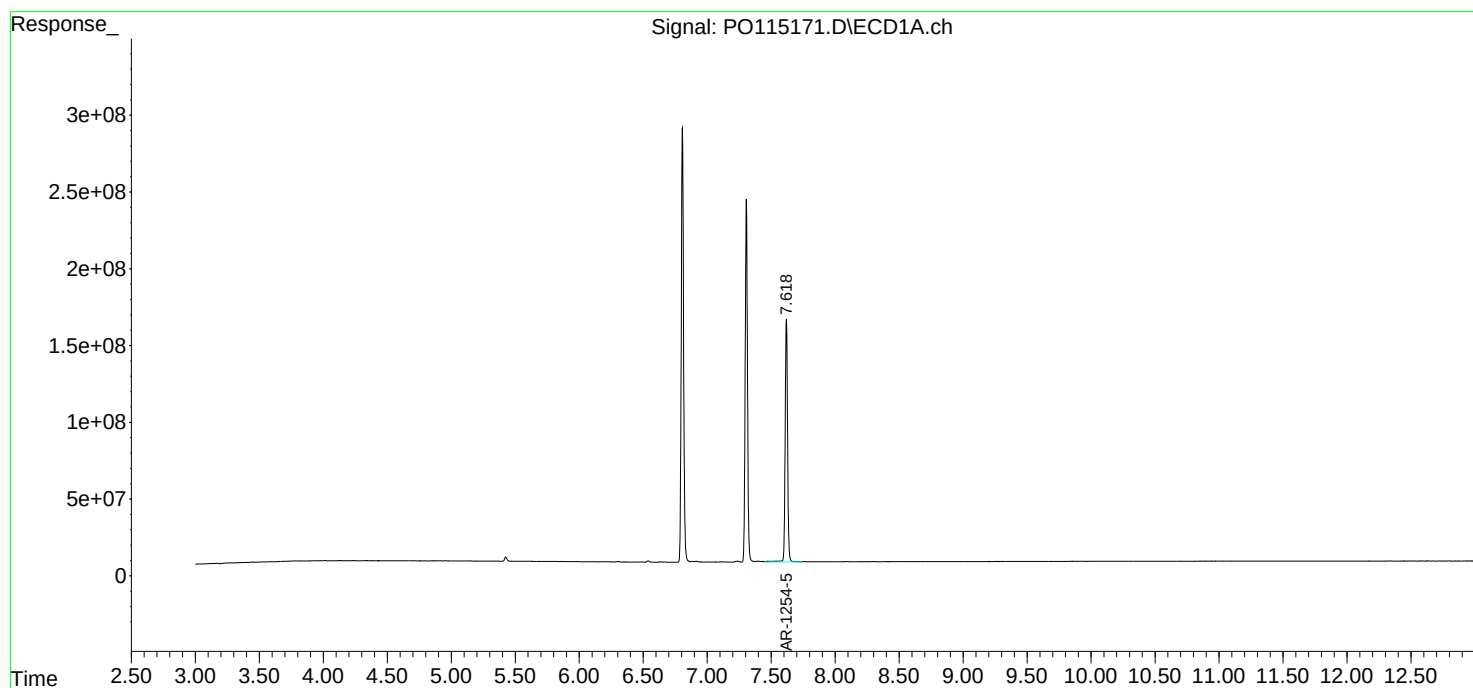

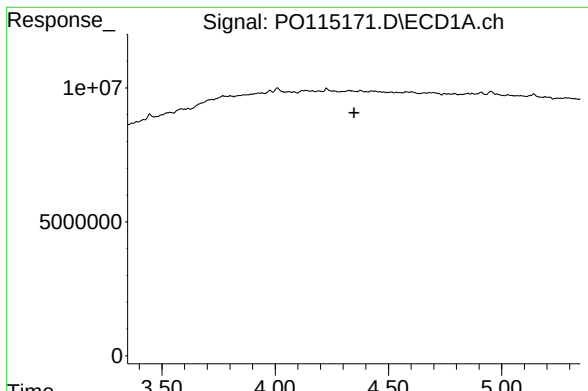

#1 Tetrachloro-m-xylene


R.T.: 0.000 min

Exp R.T. : 4.348 min

Response: 0

Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

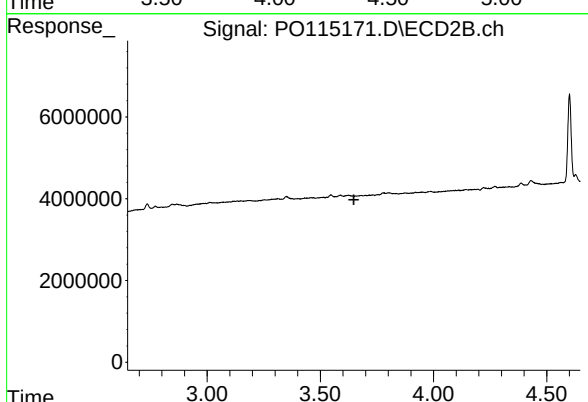


#1 Tetrachloro-m-xylene

R.T.: 0.000 min

Exp R.T. : 3.648 min

Response: 0

Conc: N.D.

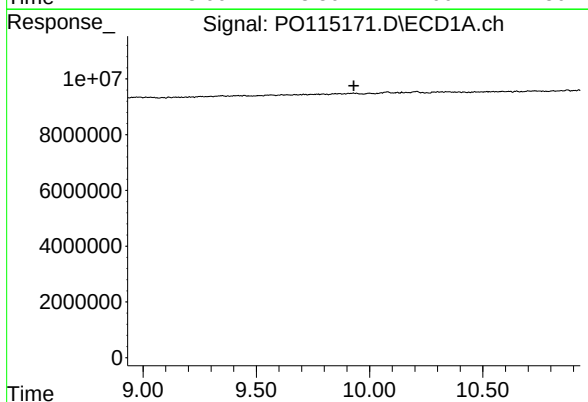


#2 Decachlorobiphenyl

R.T.: 0.000 min

Exp R.T. : 9.930 min

Response: 0

Conc: N.D.

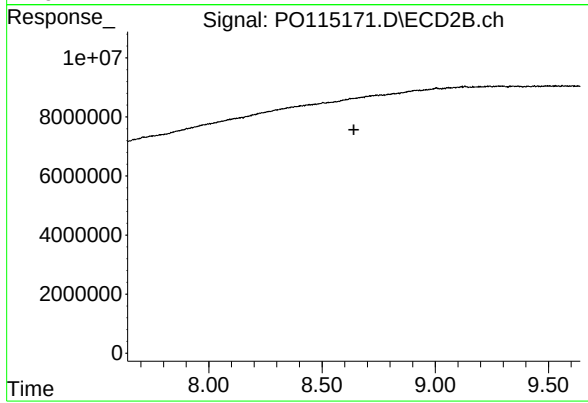


#2 Decachlorobiphenyl

R.T.: 0.000 min

Exp R.T. : 8.641 min

Response: 0


Conc: N.D.

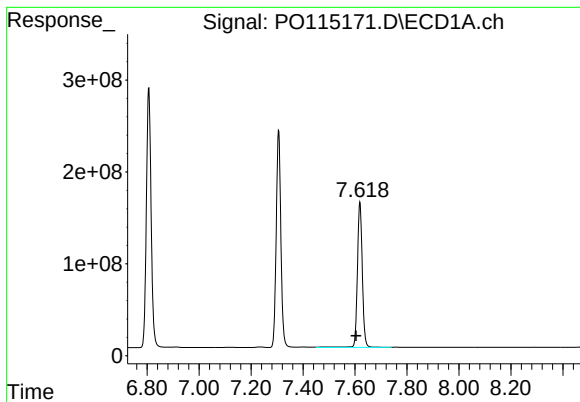

#30 AR-1254-5

R.T.: 7.619 min
Delta R.T.: 0.016 min
Response: 2086973989
Conc: 6913.87 ng/m

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

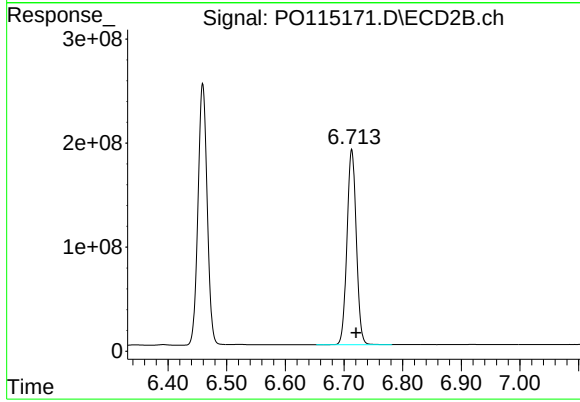

#30 AR-1254-5

R.T.: 6.713 min
Delta R.T.: -0.007 min
Response: 2074827080
Conc: 5219.35 ng/ml