

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111819\
 Data File : P0063852.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2019 19:37
 Operator : SM/AJ
 Sample : K5907-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 99K-6B

Manual Integrations
 APPROVED

Ankita
 11/19/2019 3:59:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:12:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.317	3.568	621976	445303	20.343	20.048m
2) SA Decachlor...	9.946	8.540	465024	380273	11.444	13.002

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111819\
Data File : PO063852.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2019 19:37
Operator : SM/AJ
Sample : K5907-11
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
99K-6B


Manual Integrations
APPROVED

Ankita
11/19/2019 3:59:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:12:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

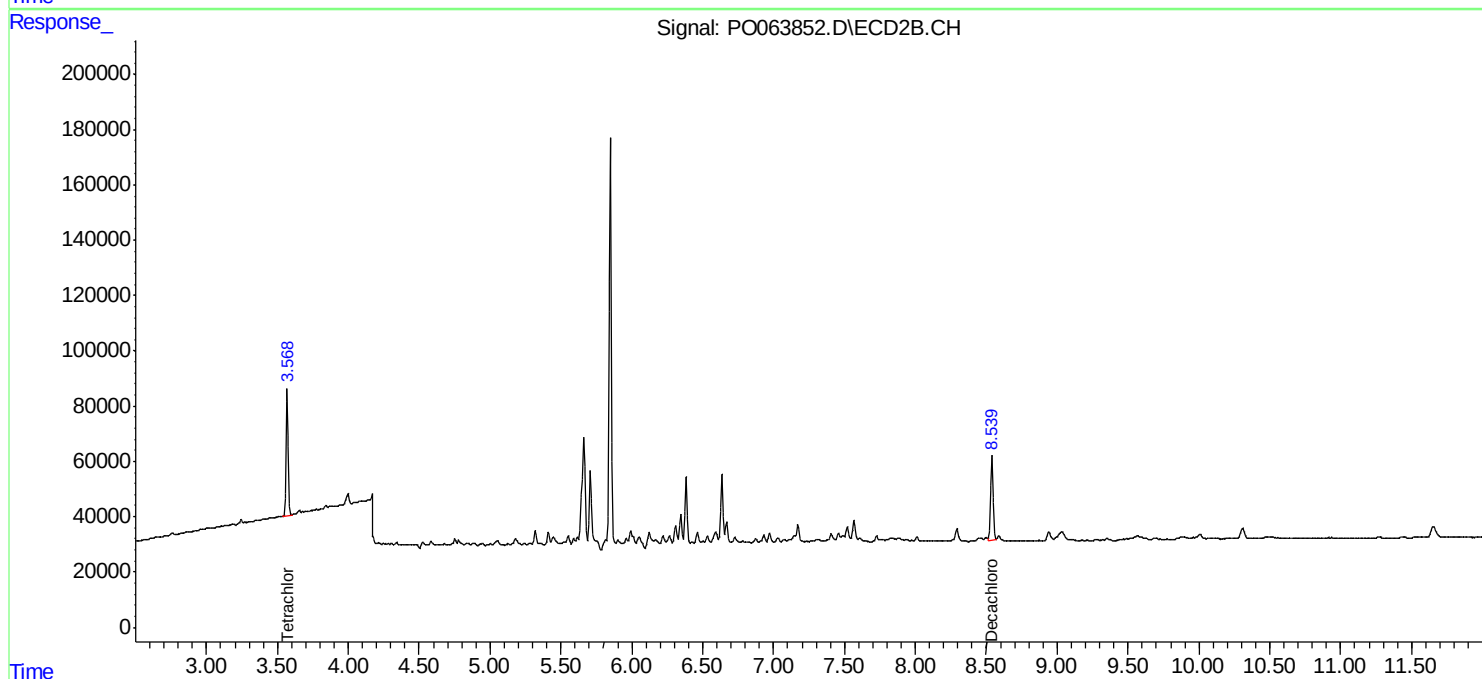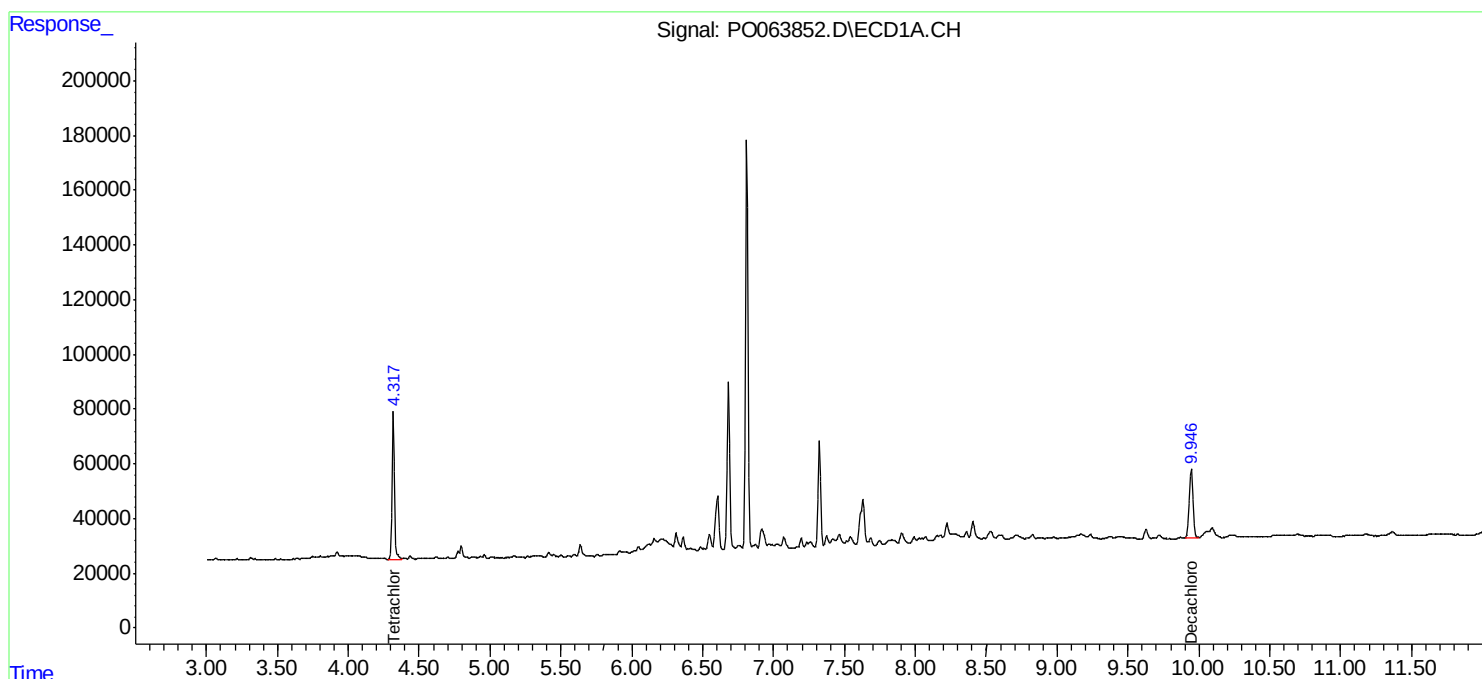

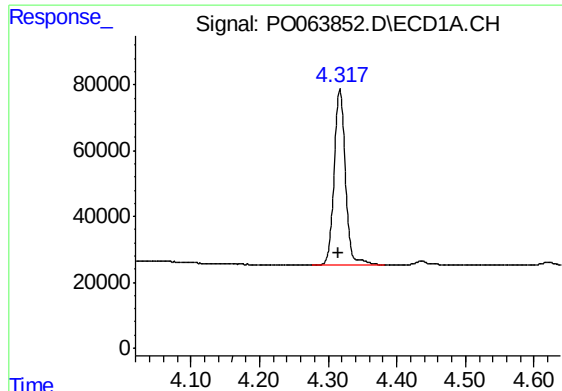


#1 Tetrachloro-m-xylene

R.T.: 4.317 min
Delta R.T.: 0.003 min
Response: 621976
Conc: 20.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
99K-6B


Manual Integrations
APPROVED

Ankita
11/19/2019 3:59:43 PM

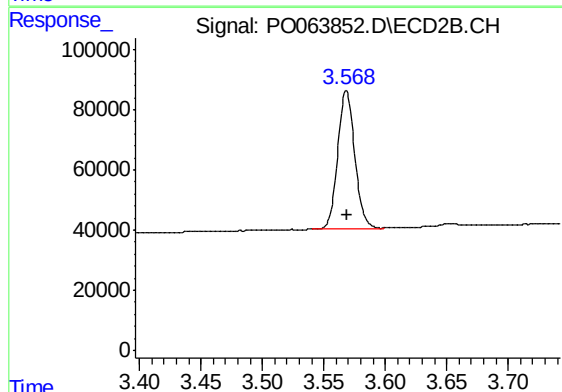


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: 0.000 min
Response: 445303
Conc: 20.05 ng/ml m

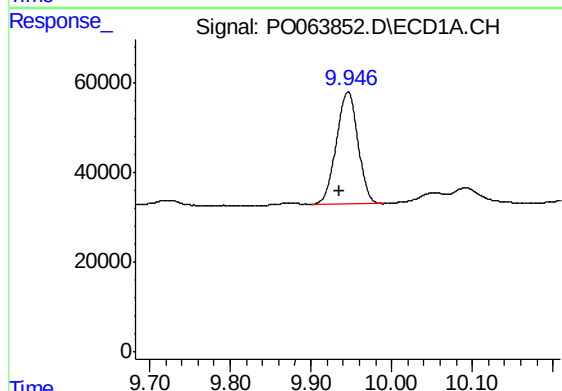

#2 Decachlorobiphenyl

R.T.: 9.946 min
Delta R.T.: 0.010 min
Response: 465024
Conc: 11.44 ng/ml

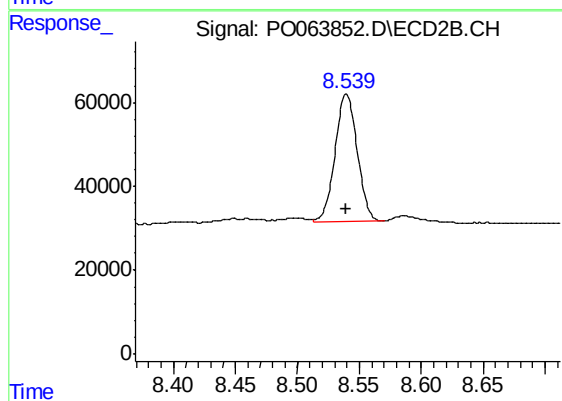

#2 Decachlorobiphenyl

R.T.: 8.540 min
Delta R.T.: 0.000 min
Response: 380273
Conc: 13.00 ng/ml