

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111819\
Data File : P0063854.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2019 20:10
Operator : SM/AJ
Sample : K5907-13
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
99K-7B

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:14:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.317	3.568	704854	506894	23.053	22.821m
2) SA Decachlor...	9.946	8.540	648706	519254	15.964	17.754

Ankita

Target Compounds

11/19/2019 3:59:46 PM

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111819\
Data File : PO063854.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2019 20:10
Operator : SM/AJ
Sample : K5907-13
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
99K-7B

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:14:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

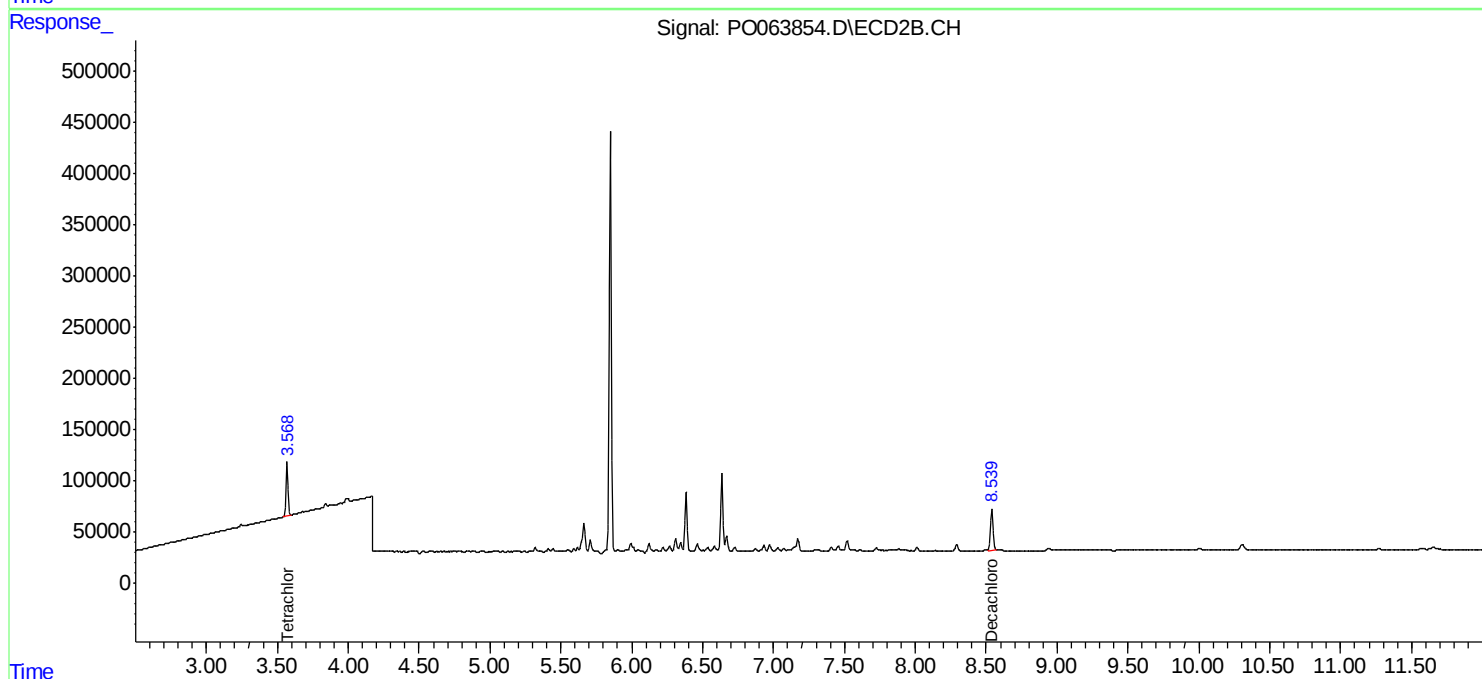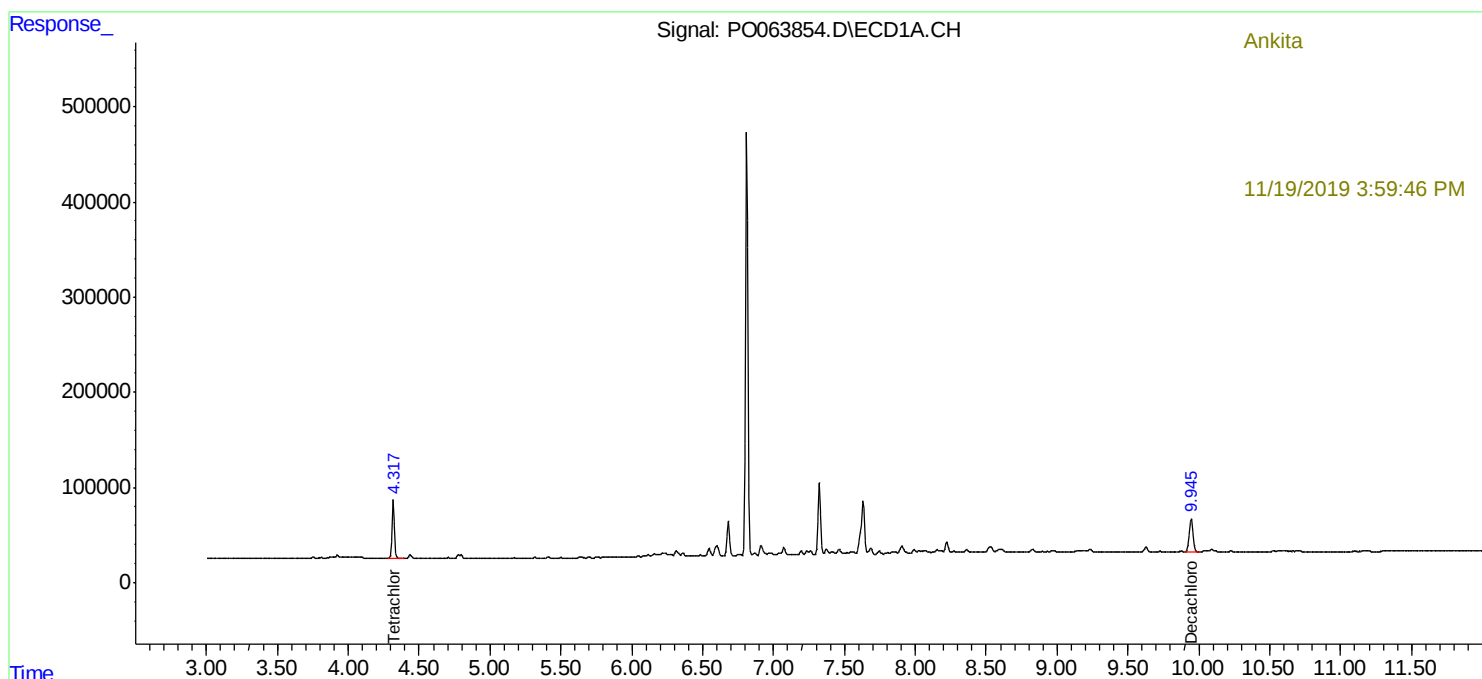

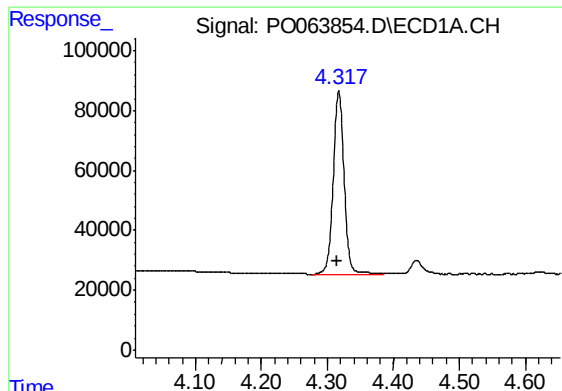


#1 Tetrachloro-m-xylene

R.T.: 4.317 min
Delta R.T.: 0.003 min
Response: 704854
Conc: 23.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
99K-7B


Manual Integrations
APPROVED

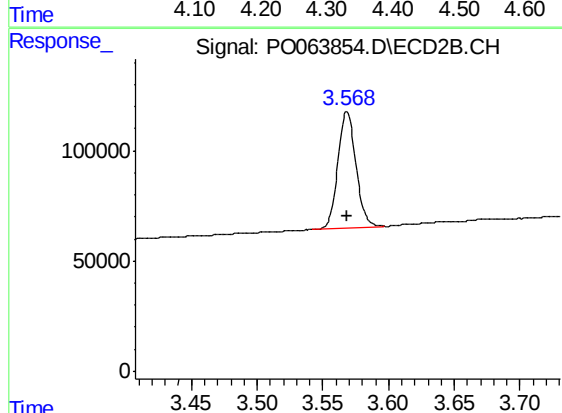

#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: 0.000 min
Response: 506894
Conc: 22.82 ng/ml m


Ankita

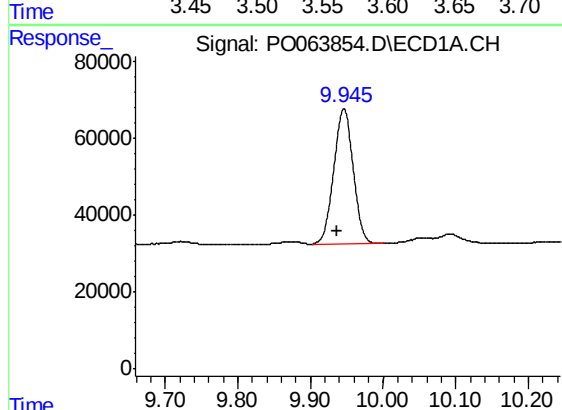

#2 Decachlorobiphenyl

R.T.: 9.946 min
Delta R.T.: 0.010 min
Response: 648706
Conc: 15.96 ng/ml

11/19/2019 3:59:46 PM

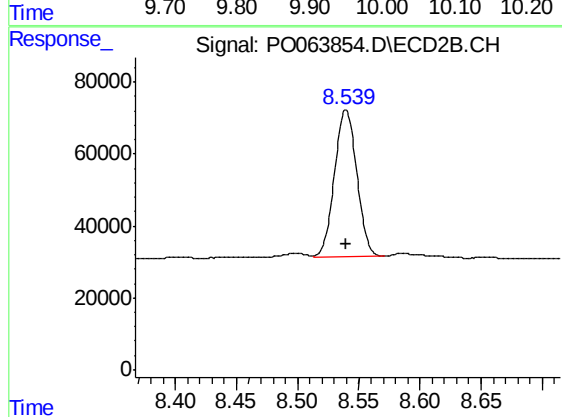

#2 Decachlorobiphenyl

R.T.: 8.540 min
Delta R.T.: 0.000 min
Response: 519254
Conc: 17.75 ng/ml