

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111820\
 Data File : PO073291.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2020 11:28
 Operator : DD\AJ
 Sample : L4766-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PIPE-AUD-31334

Manual Integrations
 APPROVED

Ankita
 11/19/2020 1:18:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 17:36:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 05:08:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.955	4.020	852104	426358	13.542	11.877m
2) SA Decachlor...	10.991	9.288	730442	495296	13.647m	14.176

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111820\
Data File : PO073291.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2020 11:28
Operator : DD\AJ
Sample : L4766-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PIPE-AUD-31334


Manual Integrations
APPROVED

Ankita
11/19/2020 1:18:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 17:36:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 05:08:01 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

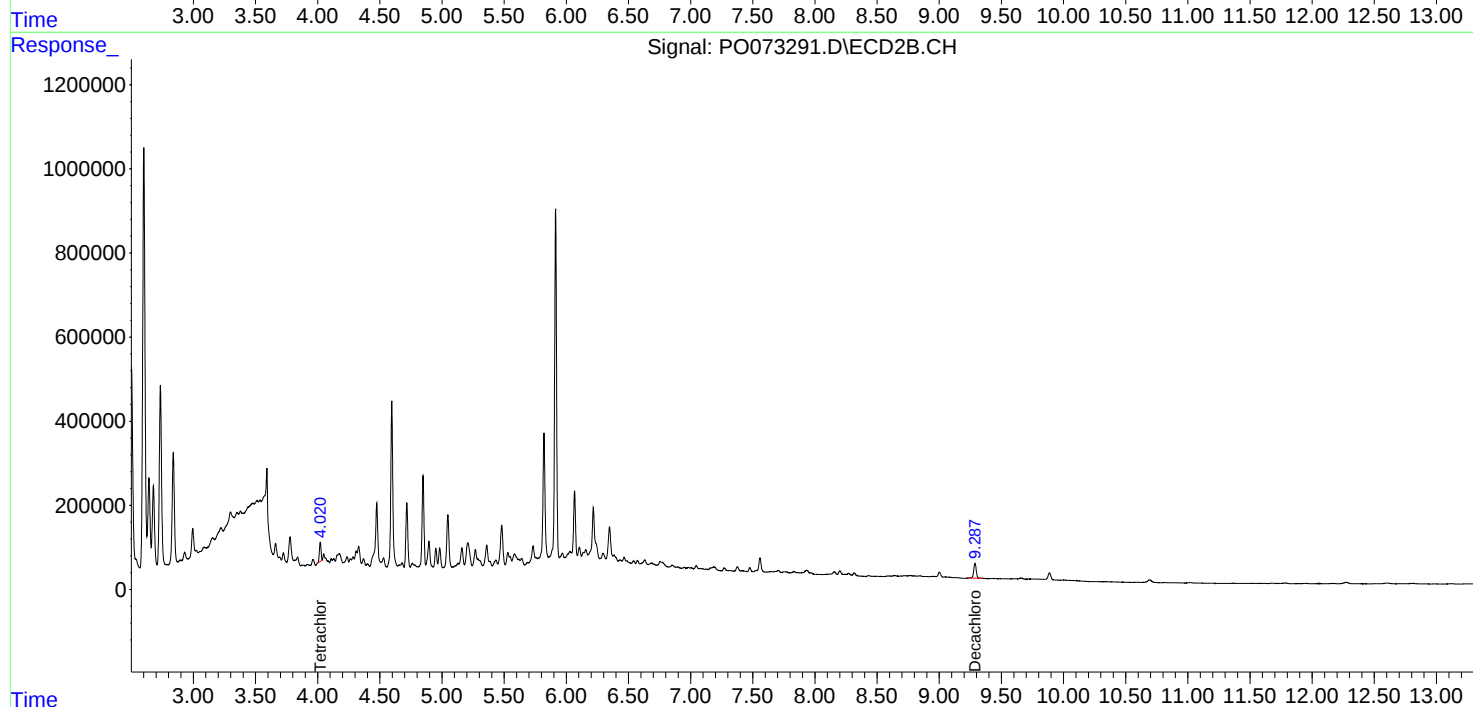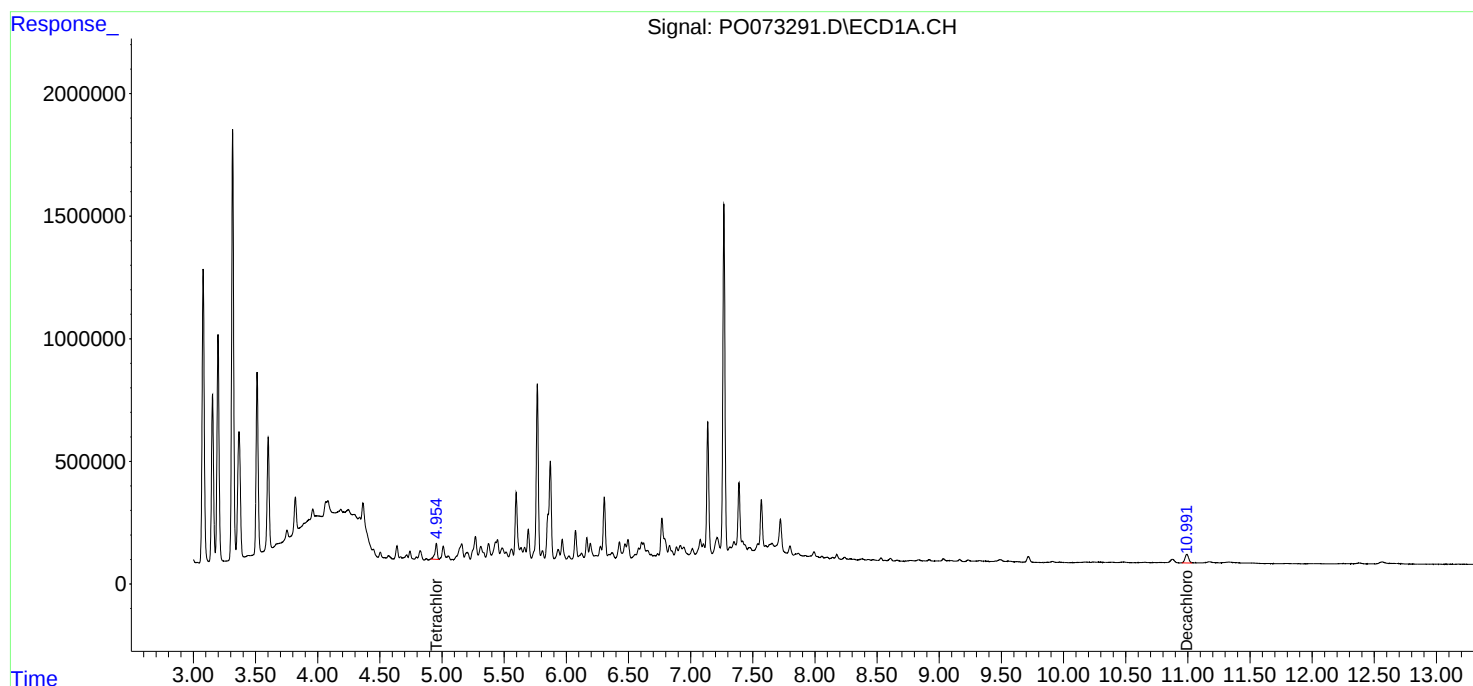

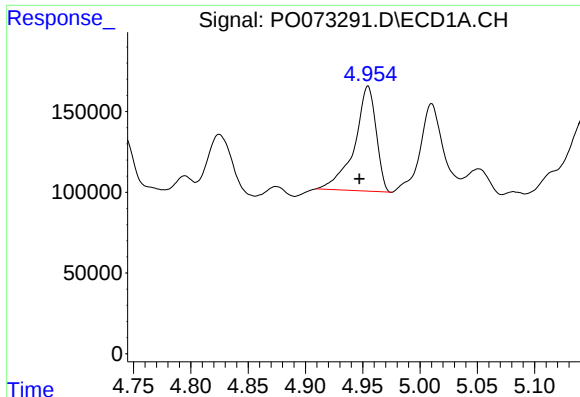


#1 Tetrachloro-m-xylene

R.T.: 4.955 min
Delta R.T.: 0.008 min
Response: 852104
Conc: 13.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIPE-AUD-31334


Manual Integrations
APPROVED

Ankita
11/19/2020 1:18:54 PM

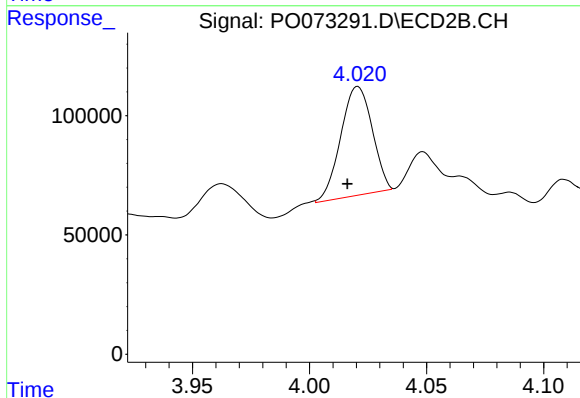


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: 0.004 min
Response: 426358
Conc: 11.88 ng/ml m

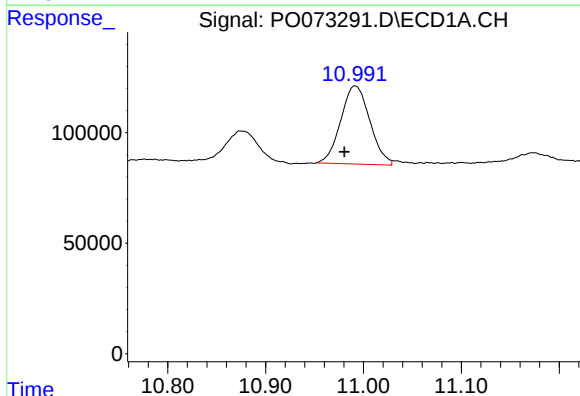

#2 Decachlorobiphenyl

R.T.: 10.991 min
Delta R.T.: 0.011 min
Response: 730442
Conc: 13.65 ng/ml m

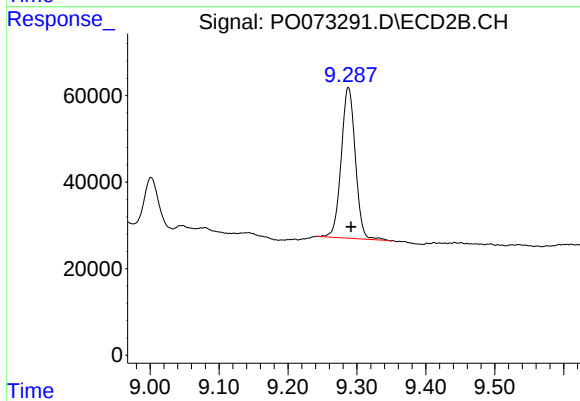

#2 Decachlorobiphenyl

R.T.: 9.288 min
Delta R.T.: -0.004 min
Response: 495296
Conc: 14.18 ng/ml