

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111820\
 Data File : PO073294.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2020 12:20
 Operator : DD\AJ
 Sample : L4742-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC-216357-LOZ-END-1-(2-1)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 17:38:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 05:08:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.950	4.017	1566774	1093385	24.899	30.458
2) SA Decachlor...	10.986	9.286	1023824	712196	19.128	20.385

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111820\
Data File : PO073294.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2020 12:20
Operator : DD\AJ
Sample : L4742-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC-216357-LOZ-END-1-(2-1)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 17:38:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 05:08:01 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

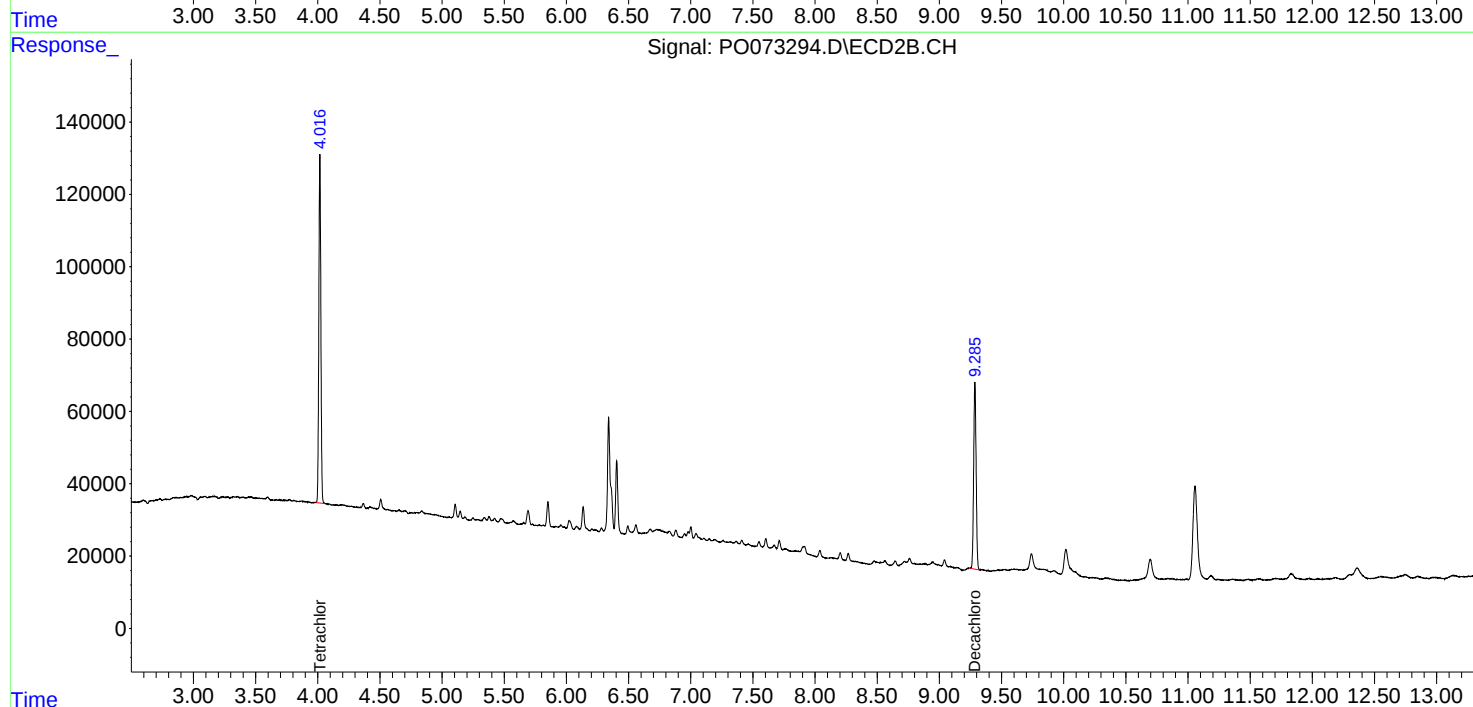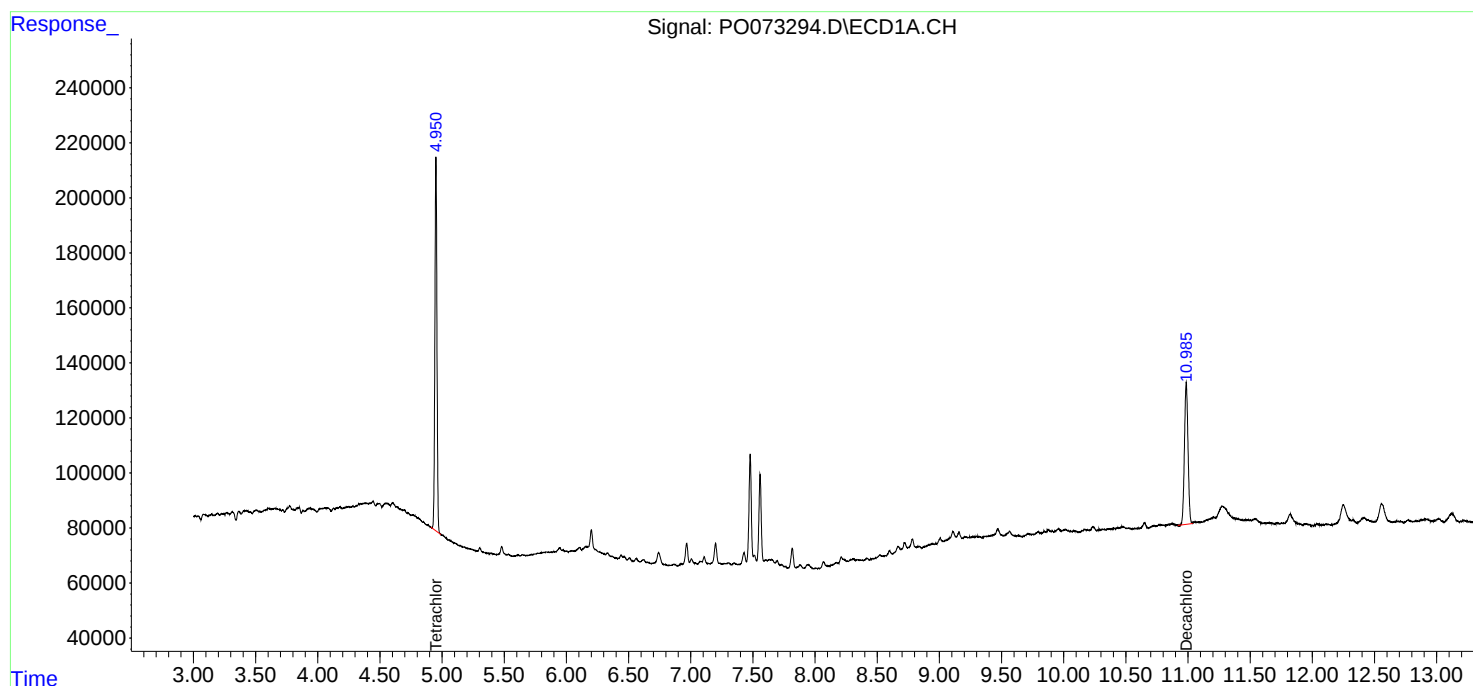


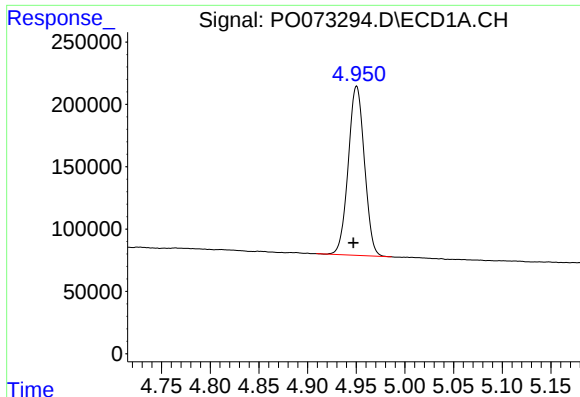

#1 Tetrachloro-m-xylene


R.T.: 4.950 min
Delta R.T.: 0.003 min
Response: 1566774
Conc: 24.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC-216357-LOZ-END-1-(2-1)

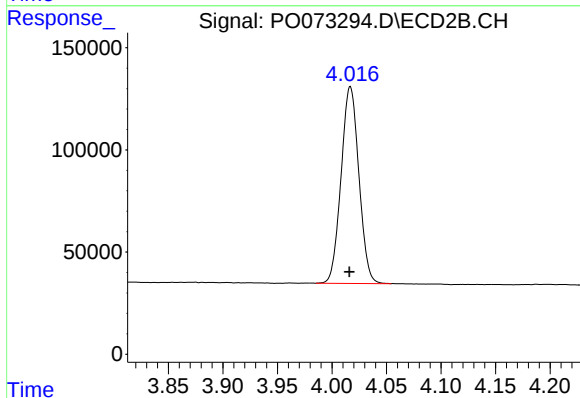


#1 Tetrachloro-m-xylene

R.T.: 4.017 min
Delta R.T.: 0.000 min
Response: 1093385
Conc: 30.46 ng/ml

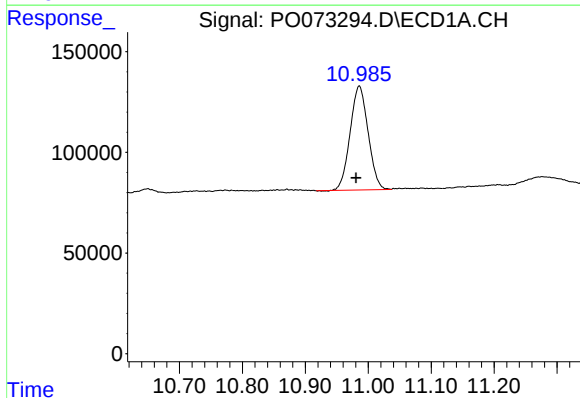

#2 Decachlorobiphenyl

R.T.: 10.986 min
Delta R.T.: 0.005 min
Response: 1023824
Conc: 19.13 ng/ml

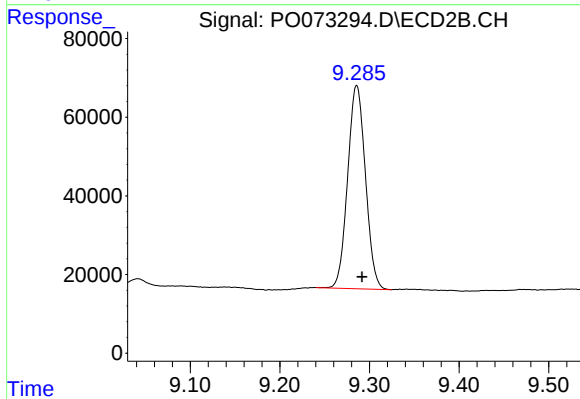

#2 Decachlorobiphenyl

R.T.: 9.286 min
Delta R.T.: -0.006 min
Response: 712196
Conc: 20.38 ng/ml