

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111820\
 Data File : PO073295.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2020 12:37
 Operator : DD\AJ
 Sample : L4742-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC-216357-LOZ-END-2-(2-2)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 17:38:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 05:08:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.954	4.019	1136594	772249	18.063	21.512
2) SA Decachlor...	10.991	9.287	896258	676220	16.745	19.355

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111820\
Data File : PO073295.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2020 12:37
Operator : DD\AJ
Sample : L4742-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC-216357-LOZ-END-2-(2-2)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 17:38:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 05:08:01 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

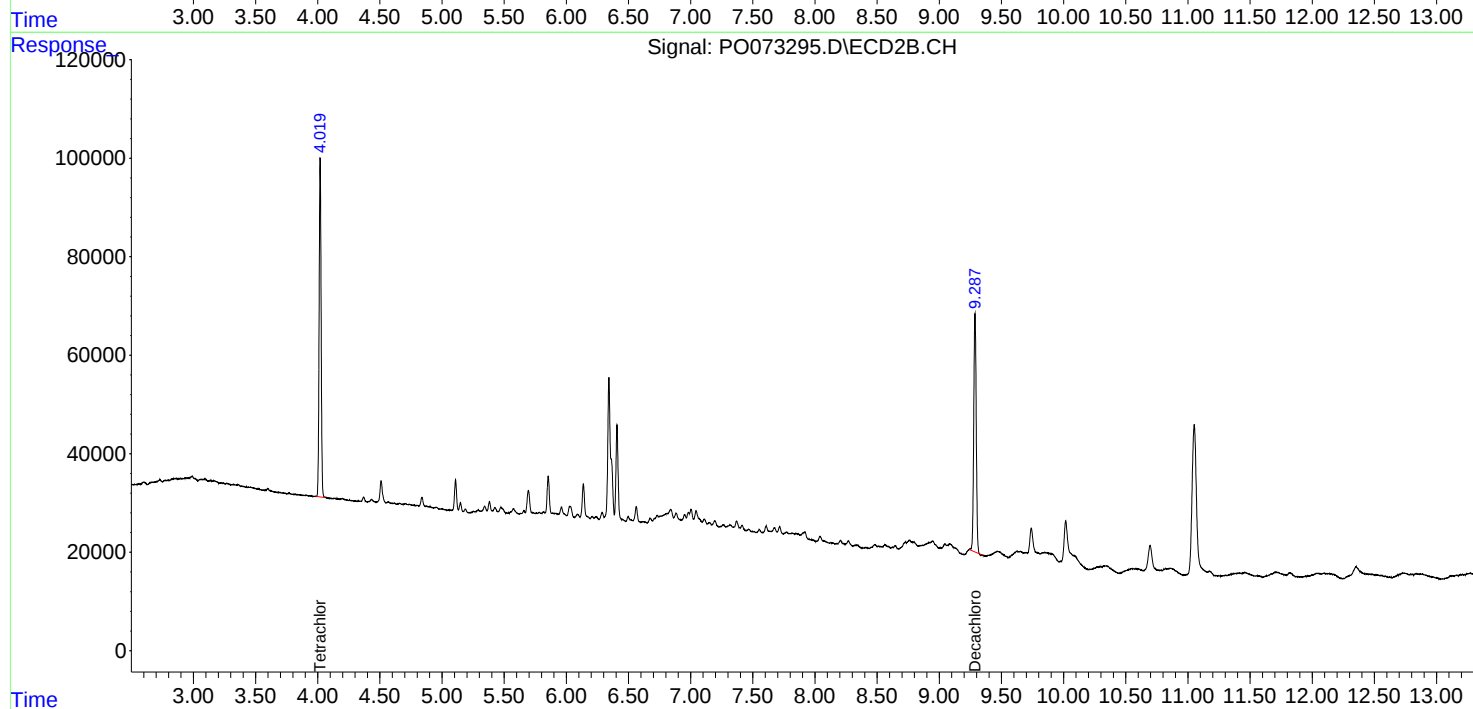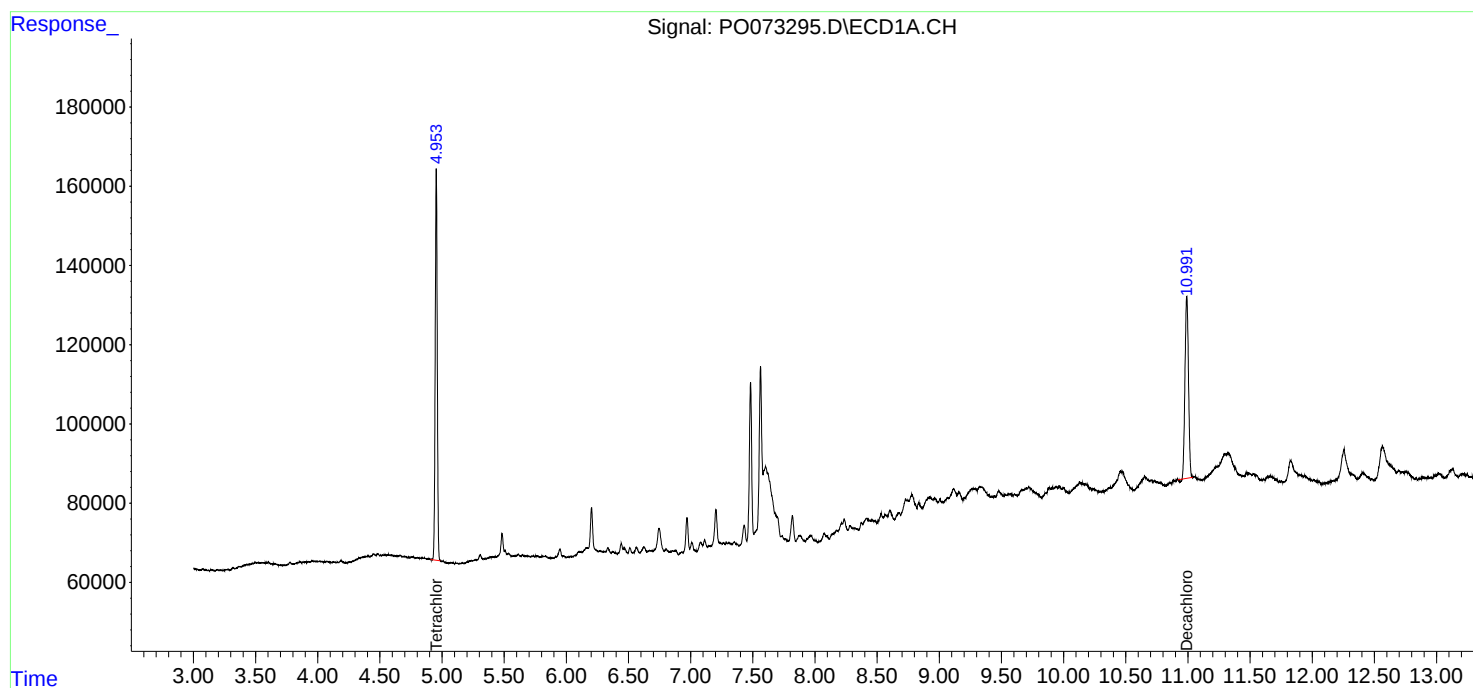


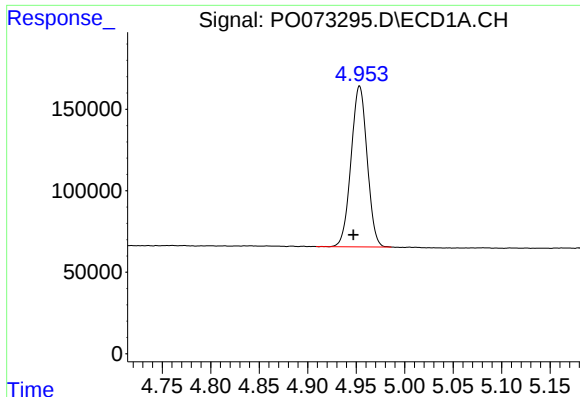

#1 Tetrachloro-m-xylene


R.T.: 4.954 min
Delta R.T.: 0.006 min
Response: 1136594
Conc: 18.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC-216357-LOZ-END-2-(2-2)

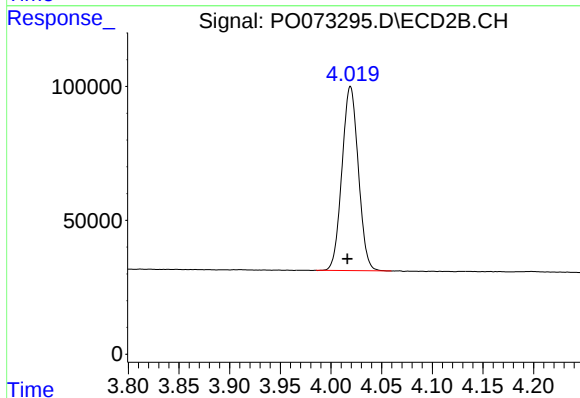


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: 0.003 min
Response: 772249
Conc: 21.51 ng/ml

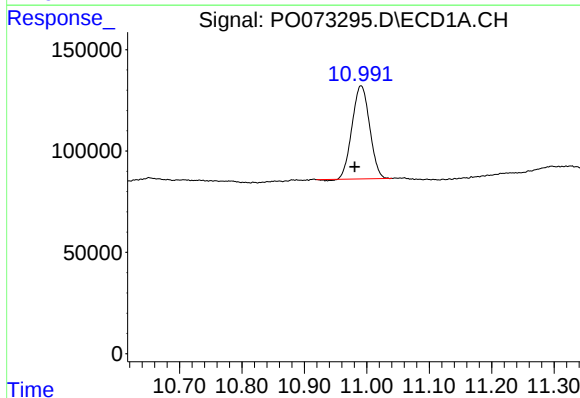

#2 Decachlorobiphenyl

R.T.: 10.991 min
Delta R.T.: 0.010 min
Response: 896258
Conc: 16.75 ng/ml

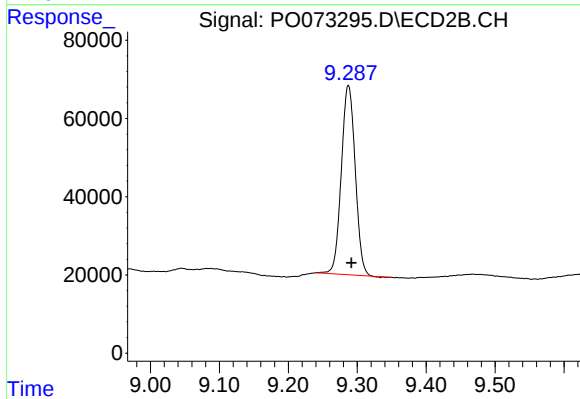

#2 Decachlorobiphenyl

R.T.: 9.287 min
Delta R.T.: -0.005 min
Response: 676220
Conc: 19.35 ng/ml