

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111821\
 Data File : PO083104.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2021 4:05
 Operator : AJ\MA
 Sample : M4728-05 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LAW-2021-5C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 05:16:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.955	3.954	141350	52542	1.585	1.619
2)	SA Decachlor...	11.044f	9.261	146126	73055	2.523	2.577
Target Compounds							
29)	L6 AR-1254-4	8.153f	0.000	26726	0	8.957	N.D. #
32)	L7 AR-1260-2	0.000	7.014	0	5498	N.D.	2.162 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111821\
Data File : PO083104.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2021 4:05
Operator : AJ\MA
Sample : M4728-05 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LAW-2021-5C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 05:16:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

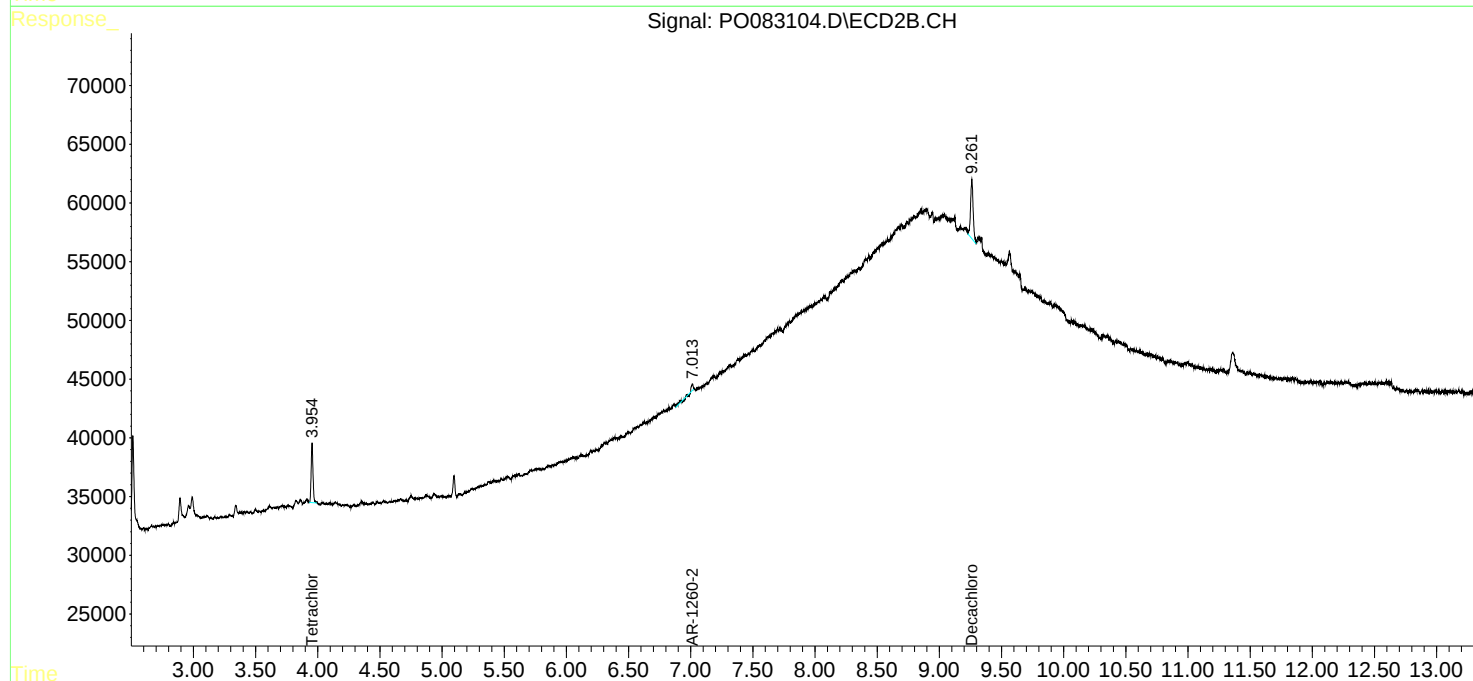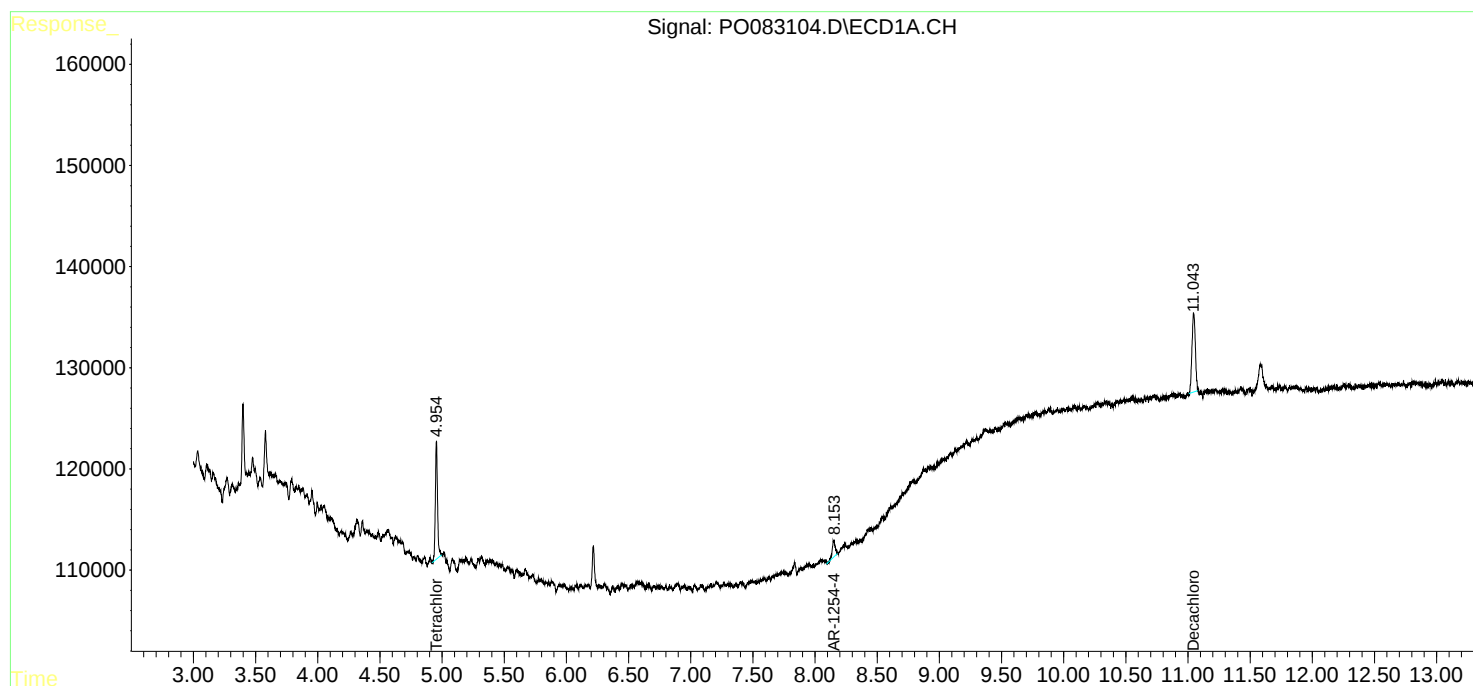


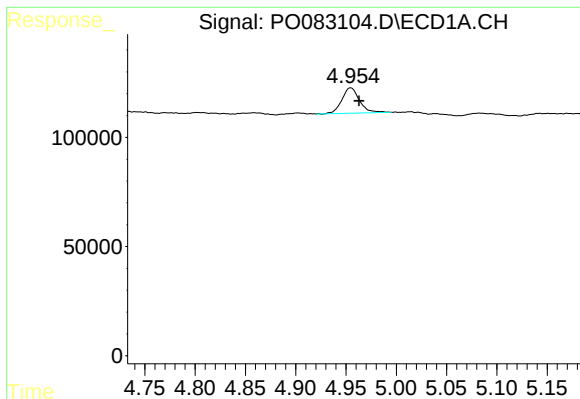

#1 Tetrachloro-m-xylene


R.T.: 4.955 min
Delta R.T.: -0.008 min
Response: 141350
Conc: 1.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LAW-2021-5C

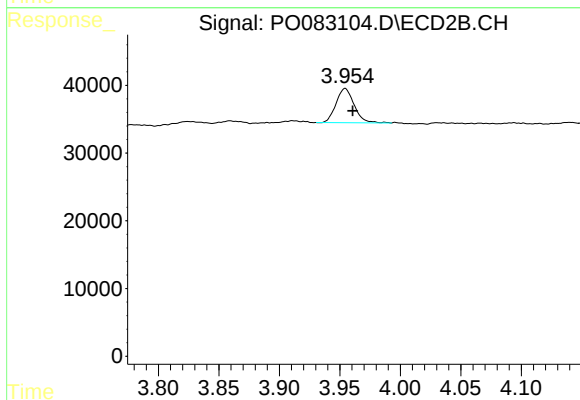


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.006 min
Response: 52542
Conc: 1.62 ng/ml

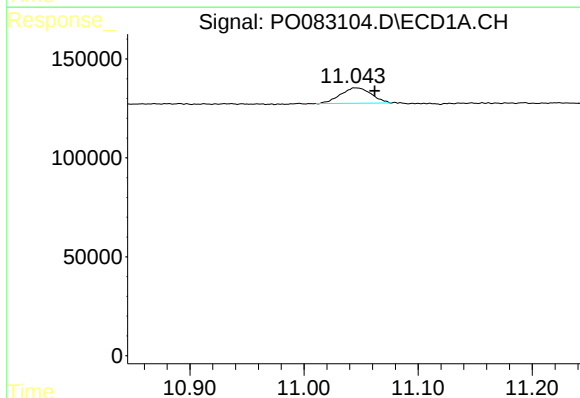


#2 Decachlorobiphenyl

R.T.: 11.044 min
Delta R.T.: -0.018 min
Response: 146126
Conc: 2.52 ng/ml

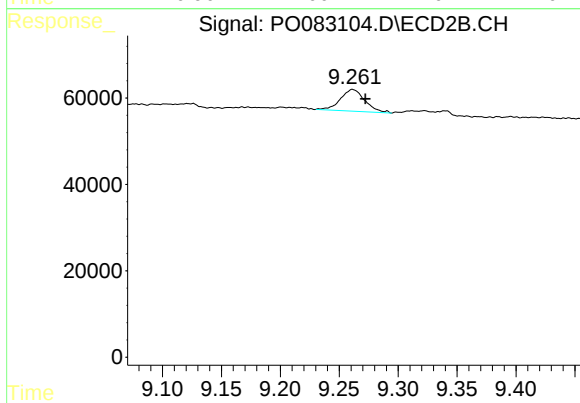

#2 Decachlorobiphenyl


R.T.: 9.261 min
Delta R.T.: -0.011 min
Response: 73055
Conc: 2.58 ng/ml

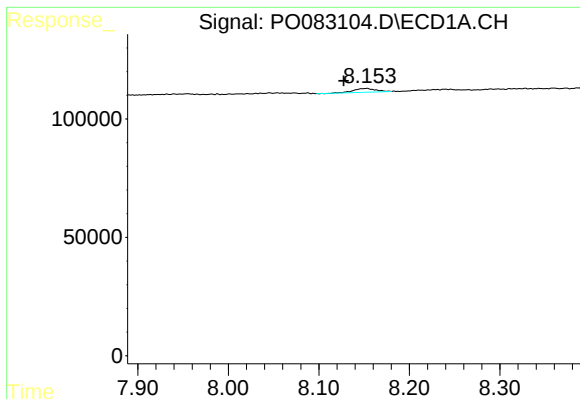

#29 AR-1254-4


R.T.: 8.153 min
Delta R.T.: 0.026 min
Response: 26726
Conc: 8.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
LAW-2021-5C

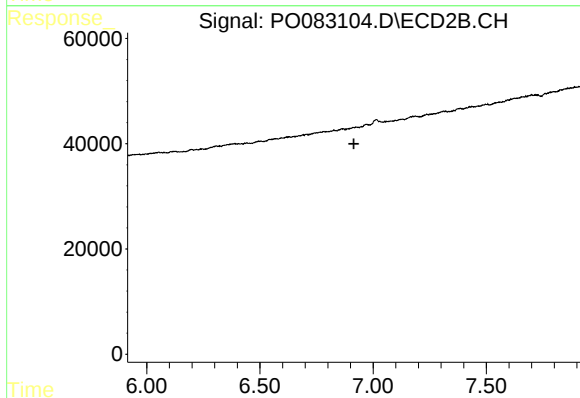


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.915 min
Response: 0
Conc: N.D.

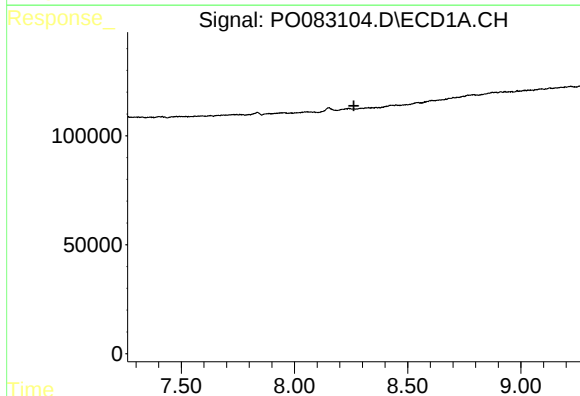

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.263 min
Response: 0
Conc: N.D.

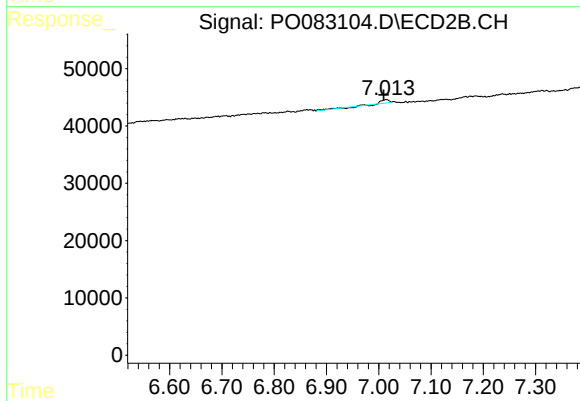

#32 AR-1260-2

R.T.: 7.014 min
Delta R.T.: 0.004 min
Response: 5498
Conc: 2.16 ng/ml