

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111821\
 Data File : PO083059.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2021 13:46
 Operator : AJ\MA
 Sample : M4724-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 3RD-FLOOR-BLOCK

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/19/2021
 Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 08:43:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.957	3.958	2107441	751413	23.634	23.157
2) SA Decachlor...	11.053	9.266	1616327	722163	27.909	25.471
Target Compounds						
31) L7 AR-1260-1	7.990	6.806	93372	95407	31.385m	49.507m#
32) L7 AR-1260-2	8.258	7.006	198675	123390	54.093m	48.516
33) L7 AR-1260-3	8.623	7.157	164527	102240	59.212m	45.959
34) L7 AR-1260-4	8.856	7.642	160122	60397	50.827	34.686 #
35) L7 AR-1260-5	9.190	7.892	268423	185017	43.333	42.245

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111821\
Data File : P0083059.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2021 13:46
Operator : AJ\MA
Sample : M4724-11
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
3RD-FLOOR-BLOCK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/19/2021
Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 08:43:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

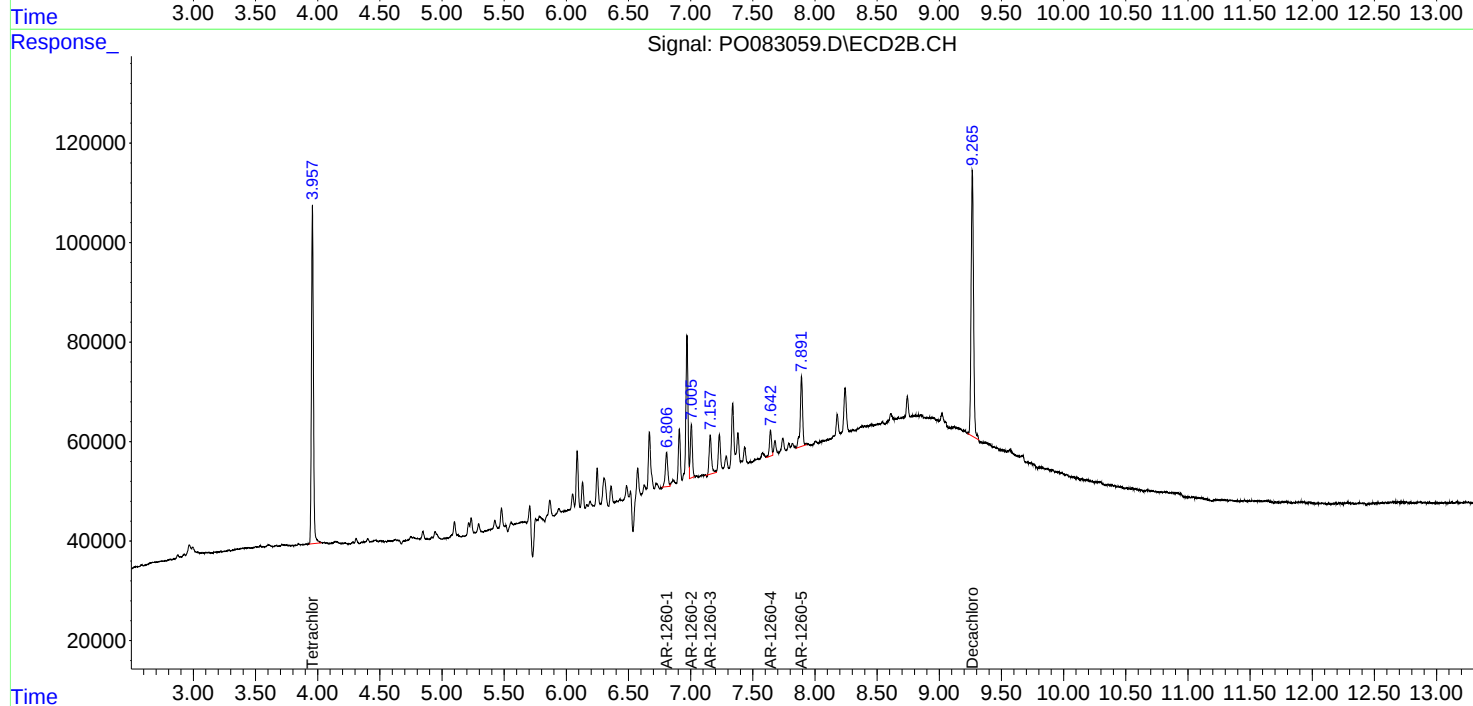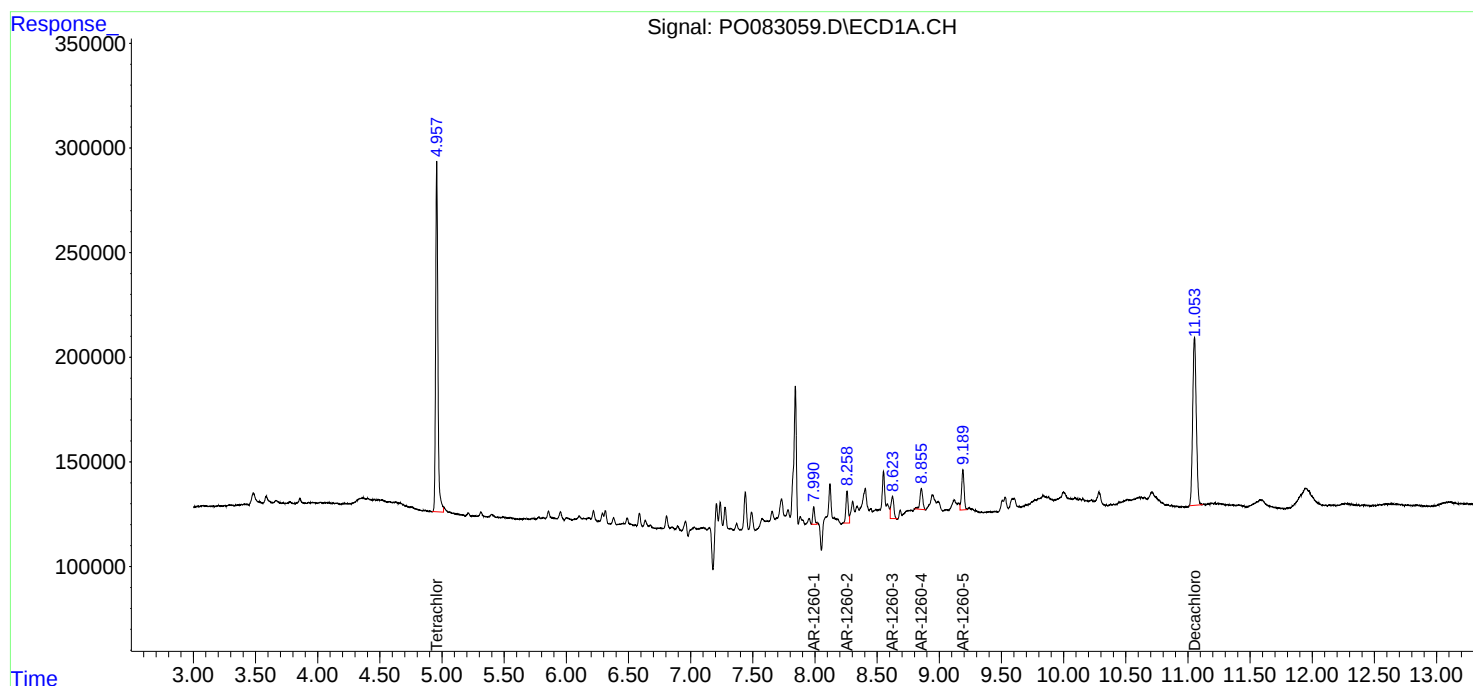

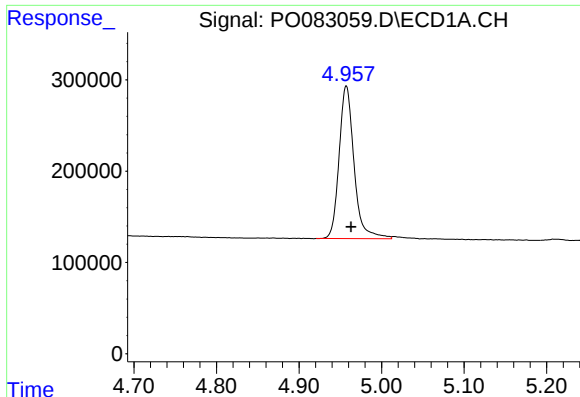


#1 Tetrachloro-m-xylene

R.T.: 4.957 min
Delta R.T.: -0.006 min
Response: 2107441
Conc: 23.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
3RD-FLOOR-BLOCK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/19/2021
Supervised By :Sohil Jodhani 11/22/2021

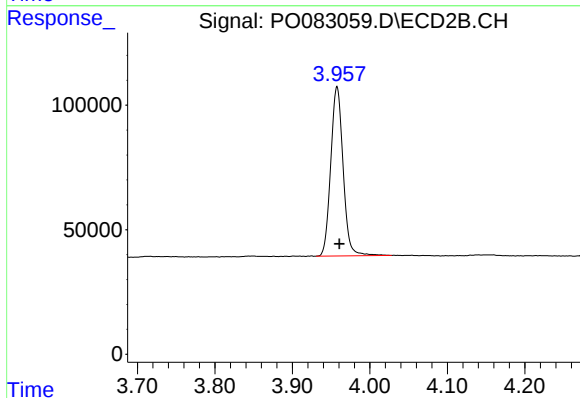


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: -0.003 min
Response: 751413
Conc: 23.16 ng/ml

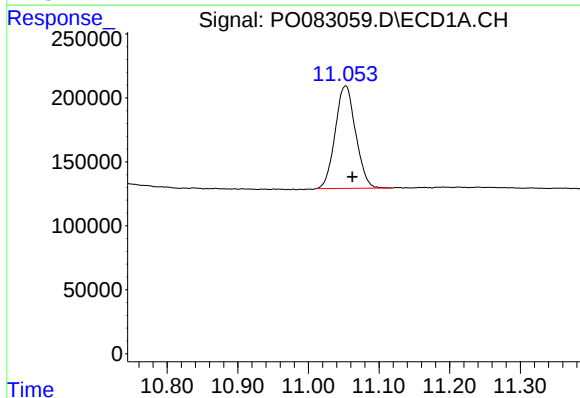


#2 Decachlorobiphenyl

R.T.: 11.053 min
Delta R.T.: -0.009 min
Response: 1616327
Conc: 27.91 ng/ml

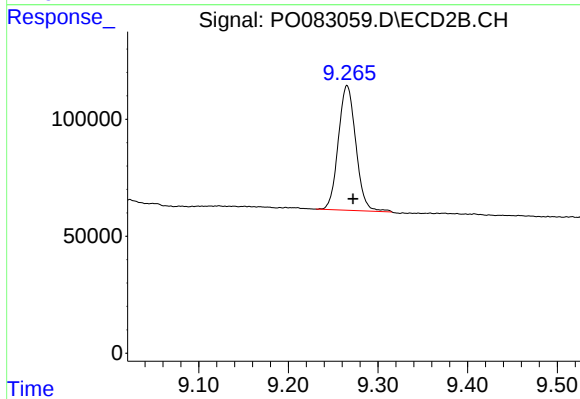

#2 Decachlorobiphenyl

R.T.: 9.266 min
Delta R.T.: -0.007 min
Response: 722163
Conc: 25.47 ng/ml

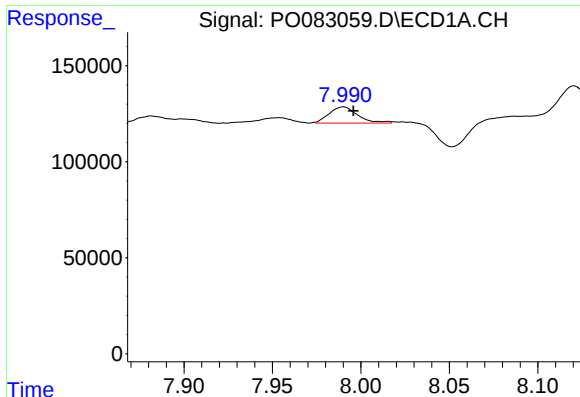


#31 AR-1260-1

R.T.: 7.990 min
Delta R.T.: -0.006 min
Response: 93372
Conc: 31.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
3RD-FLOOR-BLOCK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/19/2021
Supervised By :Sohil Jodhani 11/22/2021

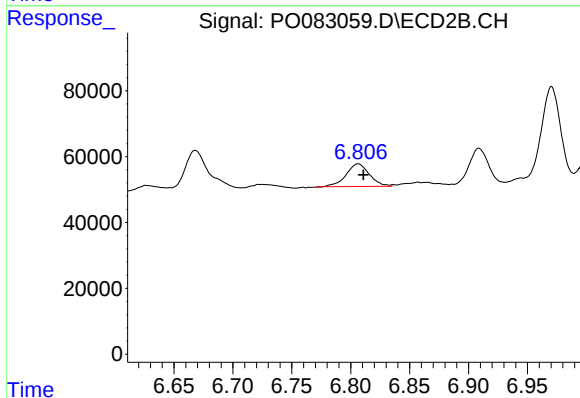


#31 AR-1260-1

R.T.: 6.806 min
Delta R.T.: -0.005 min
Response: 95407
Conc: 49.51 ng/ml m

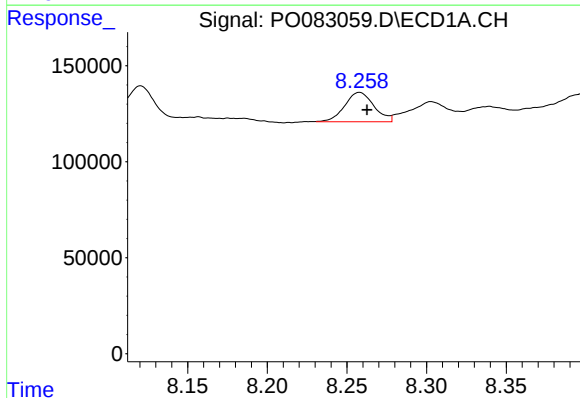


#32 AR-1260-2

R.T.: 8.258 min
Delta R.T.: -0.005 min
Response: 198675
Conc: 54.09 ng/ml m

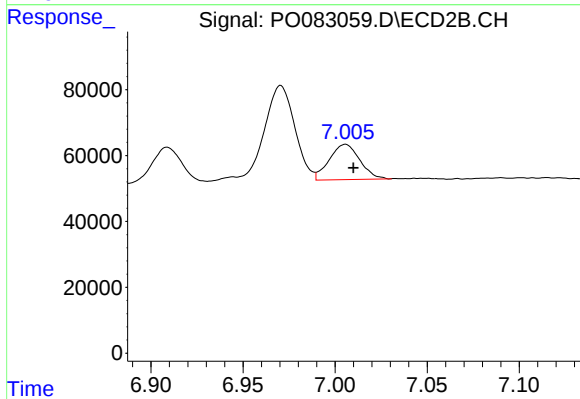

#32 AR-1260-2

R.T.: 7.006 min
Delta R.T.: -0.004 min
Response: 123390
Conc: 48.52 ng/ml

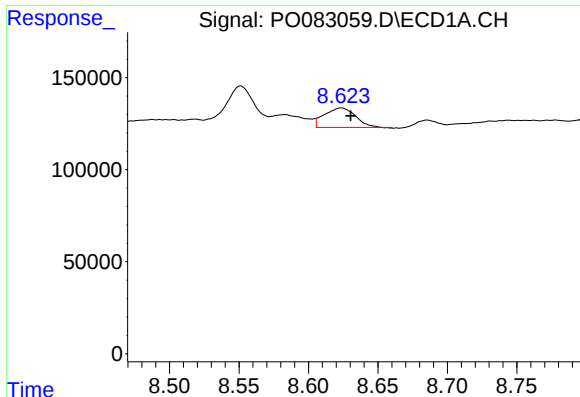


#33 AR-1260-3

R.T.: 8.623 min
Delta R.T.: -0.007 min
Response: 164527
Conc: 59.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
3RD-FLOOR-BLOCK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/19/2021
Supervised By :Sohil Jodhani 11/22/2021

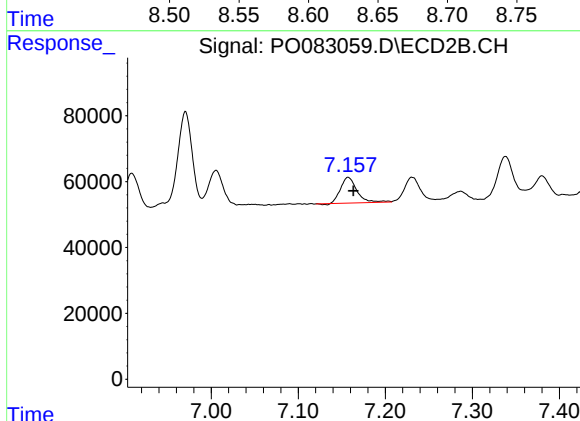


#33 AR-1260-3

R.T.: 7.157 min
Delta R.T.: -0.006 min
Response: 102240
Conc: 45.96 ng/ml

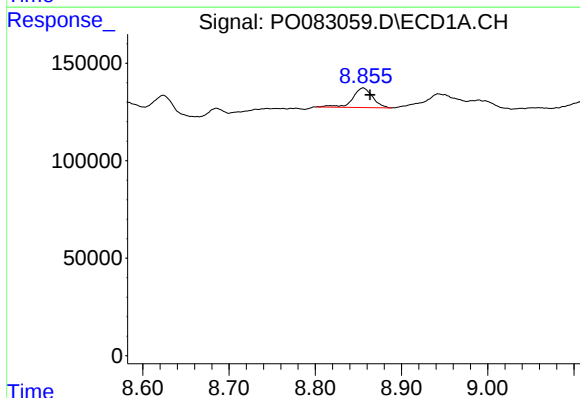


#34 AR-1260-4

R.T.: 8.856 min
Delta R.T.: -0.008 min
Response: 160122
Conc: 50.83 ng/ml

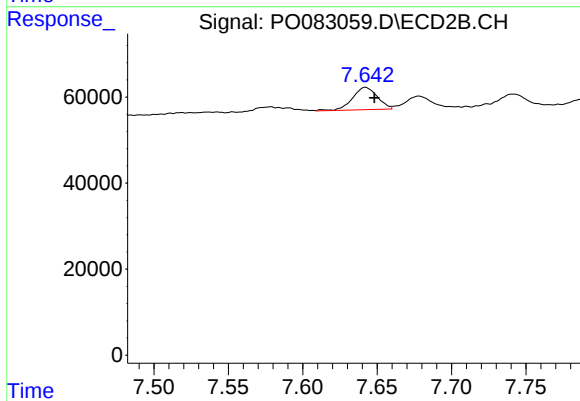

#34 AR-1260-4

R.T.: 7.642 min
Delta R.T.: -0.006 min
Response: 60397
Conc: 34.69 ng/ml

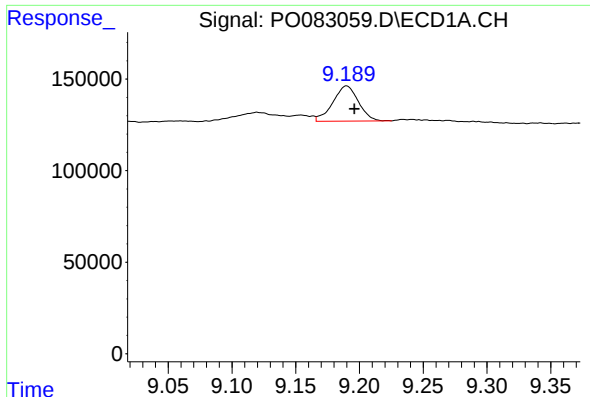

#35 AR-1260-5

R.T.: 9.190 min
Delta R.T.: -0.006 min
Response: 268423
Conc: 43.33 ng/ml


Instrument :

ECD_O

ClientSampleId :
3RD-FLOOR-BLOCK

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/19/2021
Supervised By :Sohil Jodhani 11/22/2021

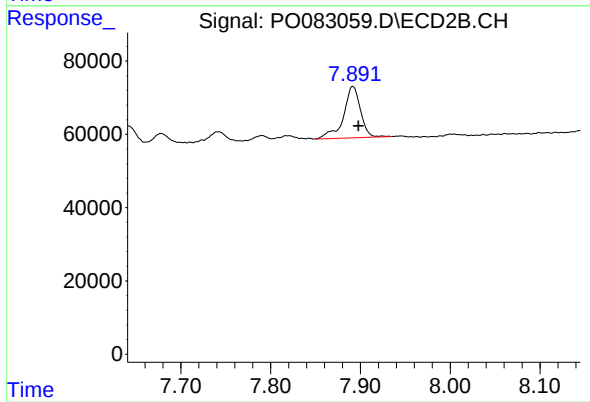

#35 AR-1260-5

R.T.: 7.892 min
Delta R.T.: -0.006 min
Response: 185017
Conc: 42.25 ng/ml