

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111821\
 Data File : PO083074.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2021 18:18
 Operator : AJ\MA
 Sample : M4731-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 C-1600-FLOOD-WALL-JG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 04:59:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.958	3.957	1723938	604704	19.333	18.636
2) SA Decachlor...	11.054	9.266	992563	803077	17.138	28.324 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111821\
Data File : P0083074.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2021 18:18
Operator : AJ\MA
Sample : M4731-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
C-1600-FLOOD-WALL-JG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 04:59:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

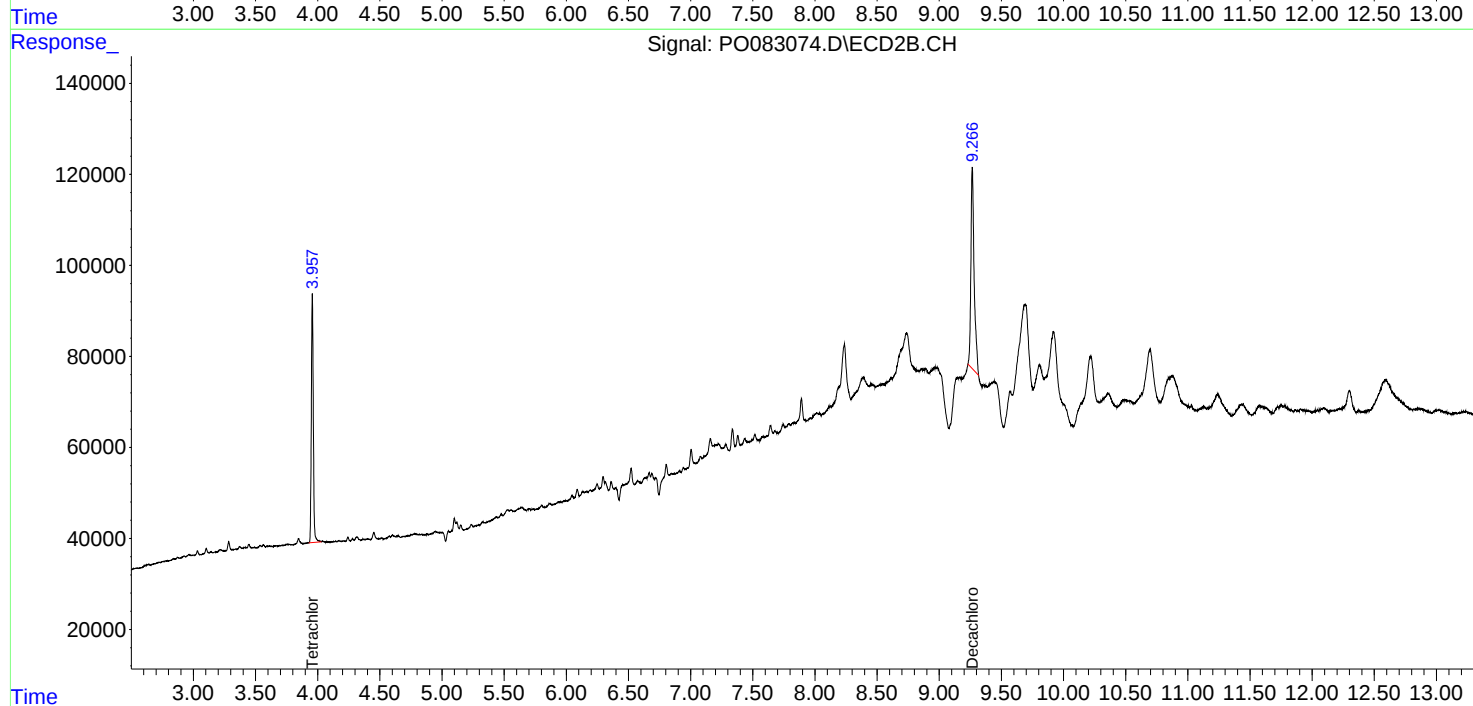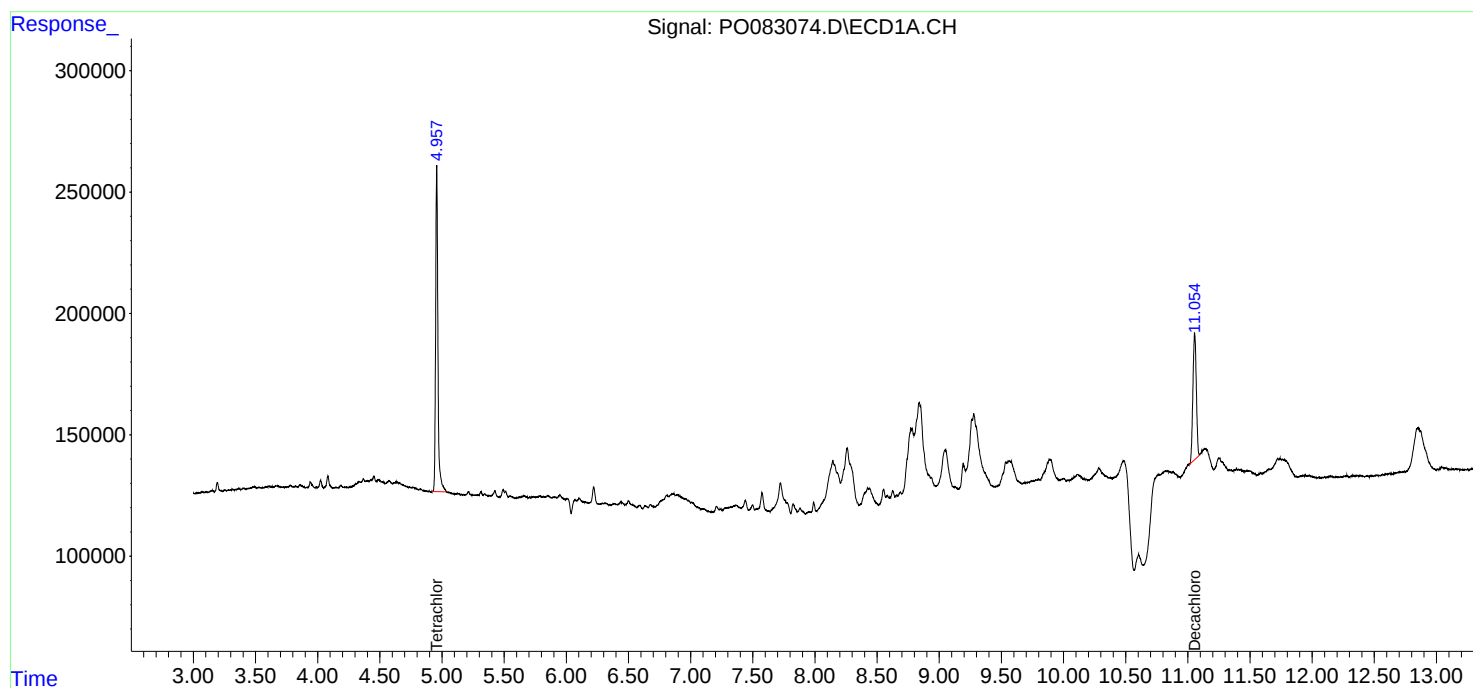


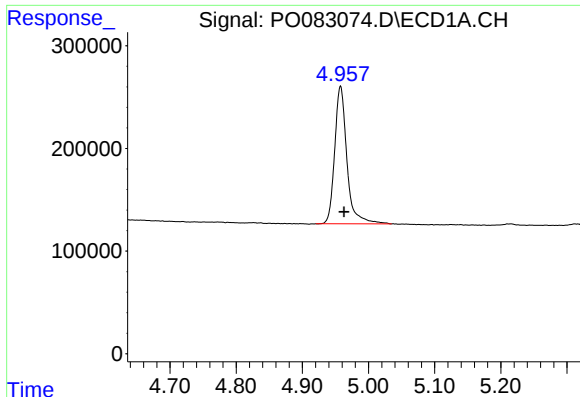

#1 Tetrachloro-m-xylene


R.T.: 4.958 min
Delta R.T.: -0.005 min
Response: 1723938
Conc: 19.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
C-1600-FLOOD-WALL-JG

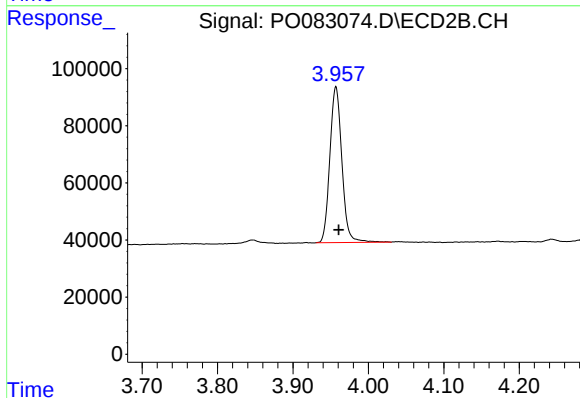


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.004 min
Response: 604704
Conc: 18.64 ng/ml

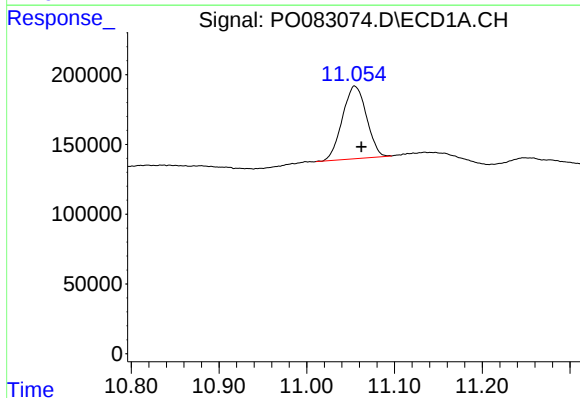

#2 Decachlorobiphenyl

R.T.: 11.054 min
Delta R.T.: -0.008 min
Response: 992563
Conc: 17.14 ng/ml

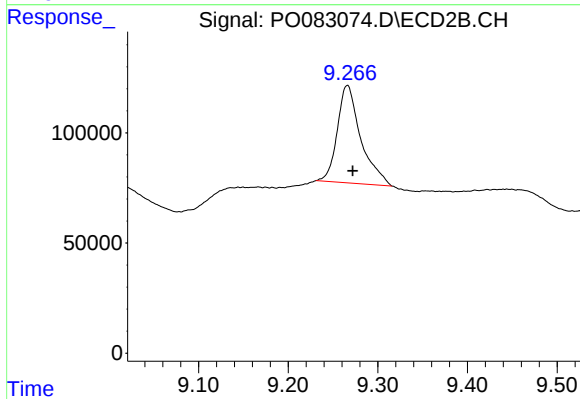

#2 Decachlorobiphenyl

R.T.: 9.266 min
Delta R.T.: -0.006 min
Response: 803077
Conc: 28.32 ng/ml