

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111821\
 Data File : PO083075.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2021 18:35
 Operator : AJ\MA
 Sample : M4732-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 33536

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/19/2021
 Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 05:00:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.962	3.966	1022709	496109	11.469m	15.289 #
2) SA Decachlor...	11.069	9.281	1128250	430705	19.481	15.191

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111821\
Data File : PO083075.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2021 18:35
Operator : AJ\MA
Sample : M4732-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
33536


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/19/2021
Supervised By :Sohil Jodhani 11/22/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 05:00:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

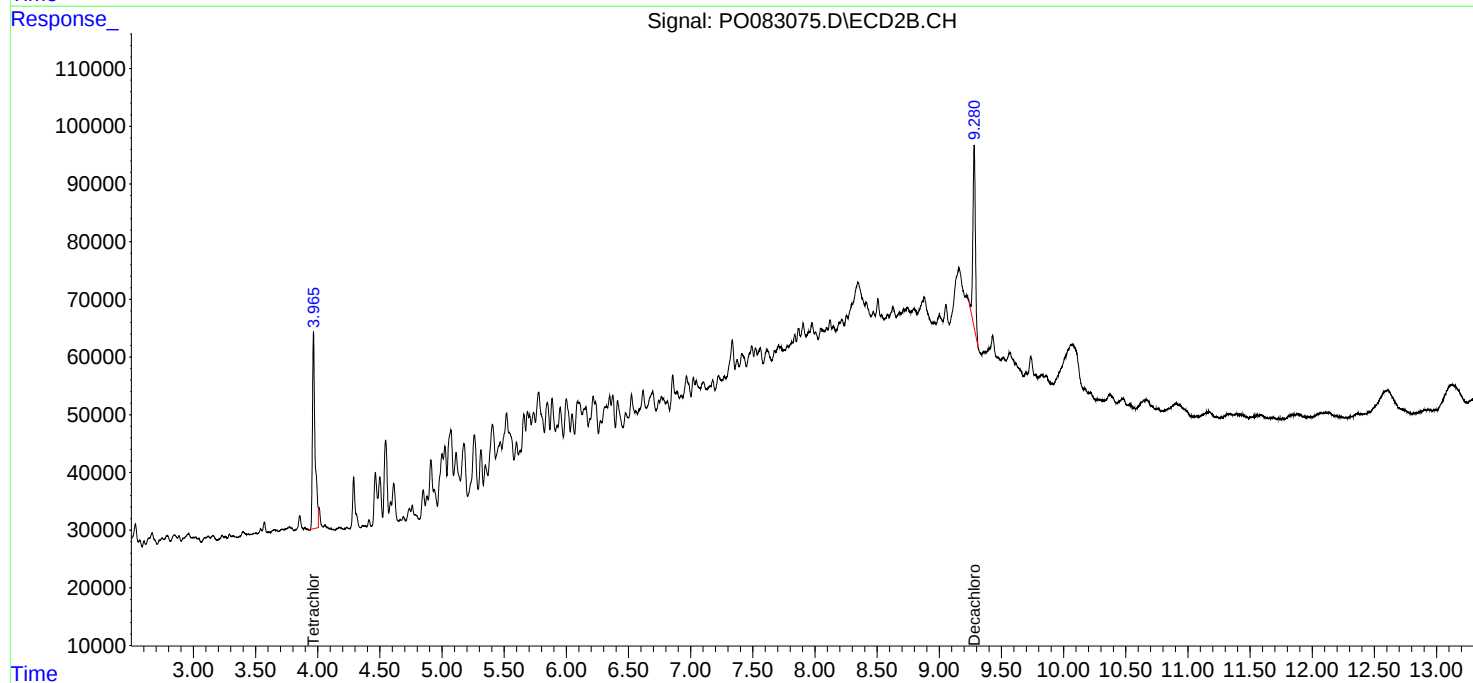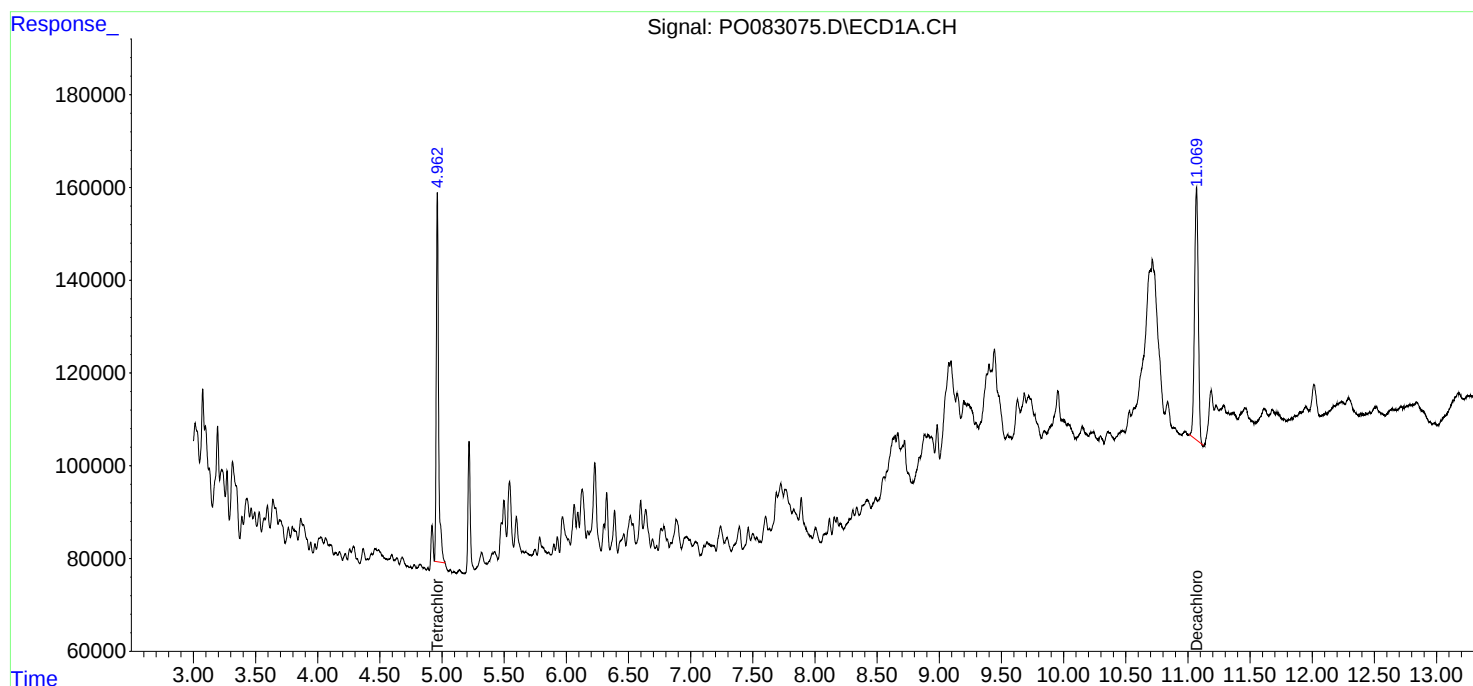

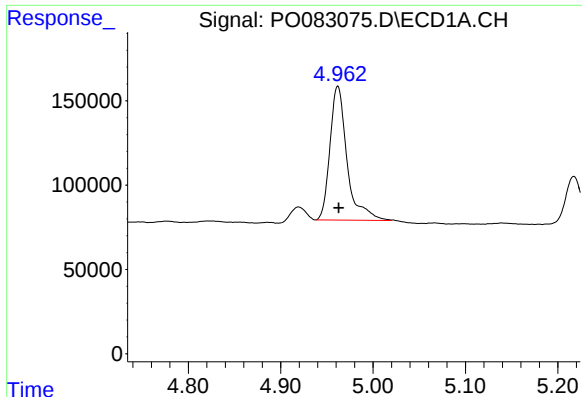


#1 Tetrachloro-m-xylene

R.T.: 4.962 min
Delta R.T.: -0.001 min
Response: 1022709
Conc: 11.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
33536


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/19/2021
Supervised By :Sohil Jodhani 11/22/2021

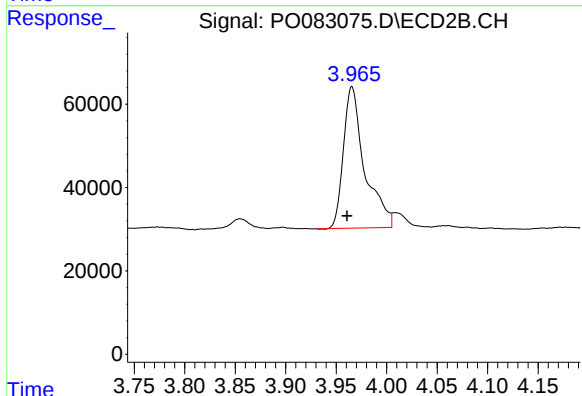


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.005 min
Response: 496109
Conc: 15.29 ng/ml

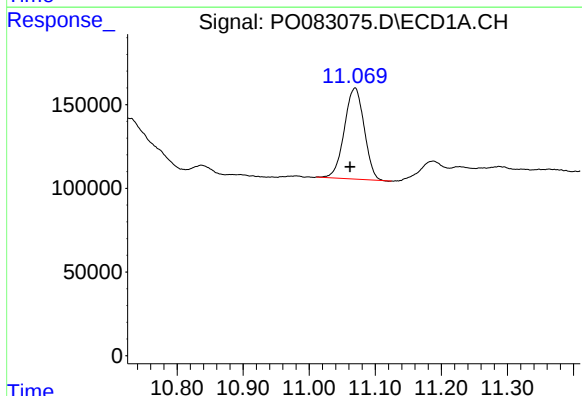

#2 Decachlorobiphenyl

R.T.: 11.069 min
Delta R.T.: 0.007 min
Response: 1128250
Conc: 19.48 ng/ml

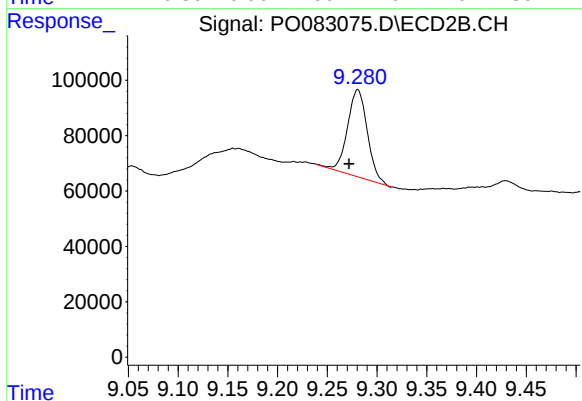

#2 Decachlorobiphenyl

R.T.: 9.281 min
Delta R.T.: 0.009 min
Response: 430705
Conc: 15.19 ng/ml