

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111822\
 Data File : P0090753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2022 10:50
 Operator : YP/AJ
 Sample : N5675-08RE 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AUD-1245RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/21/2022
 Supervised By :Ankita Jodhani 11/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 16:02:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.297	3.477	2602677	1659119	0.810m	1.561m#
2) SA Decachlor...	10.053	8.477	78897946	4395852	32.196m	4.268 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111822\
Data File : PO090753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2022 10:50
Operator : YP/AJ
Sample : N5675-08RE 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
AUD-1245RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2022
Supervised By :Ankita Jodhani 11/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 16:02:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

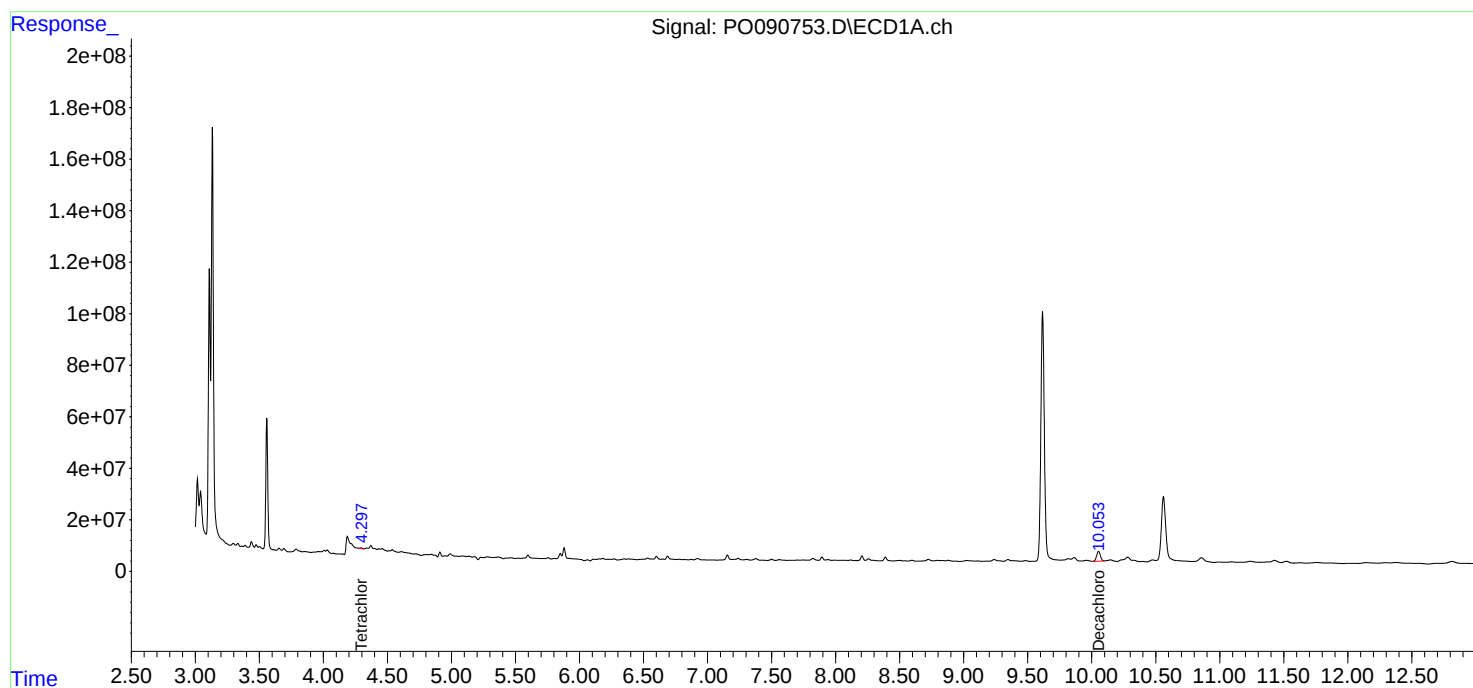

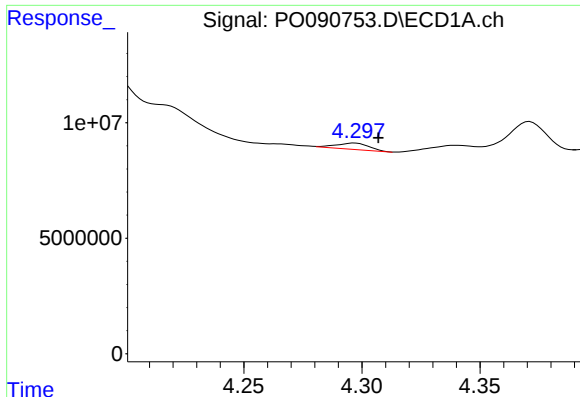


#1 Tetrachloro-m-xylene

R.T.: 4.297 min
Delta R.T.: -0.010 min
Response: 2602677
Conc: 0.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1245RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2022
Supervised By :Ankita Jodhani 11/21/2022

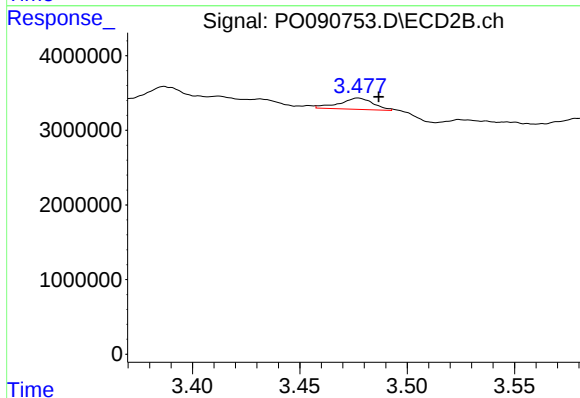


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: -0.010 min
Response: 1659119
Conc: 1.56 ng/ml m

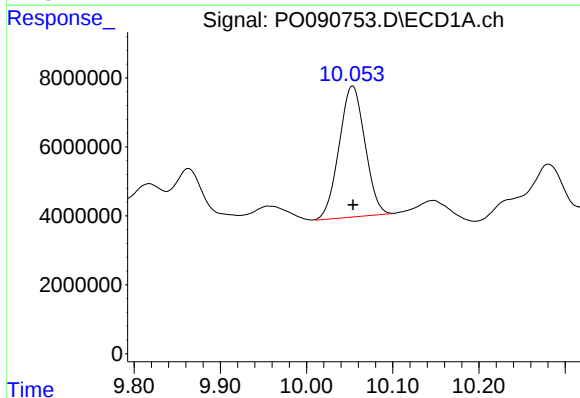

#2 Decachlorobiphenyl

R.T.: 10.053 min
Delta R.T.: 0.000 min
Response: 78897946
Conc: 32.20 ng/ml m

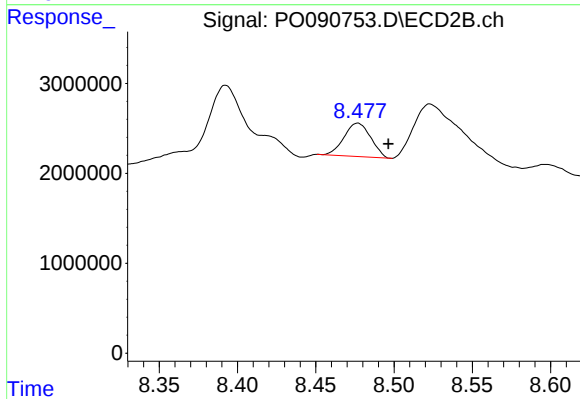

#2 Decachlorobiphenyl

R.T.: 8.477 min
Delta R.T.: -0.020 min
Response: 4395852
Conc: 4.27 ng/ml