

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111822\
 Data File : PO090798.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2022 05:11
 Operator : YP/AJ
 Sample : N5678-15
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 250FB-BP-BACKFILL-08

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 08:16:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.298	3.477	79338837	24998667	24.686	23.522
2) SA Decachlor...	10.047	8.479	57913707	22116056	23.633	21.473

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111822\
Data File : PO090798.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2022 05:11
Operator : YP/AJ
Sample : N5678-15
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
250FB-BP-BACKFILL-08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 08:16:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

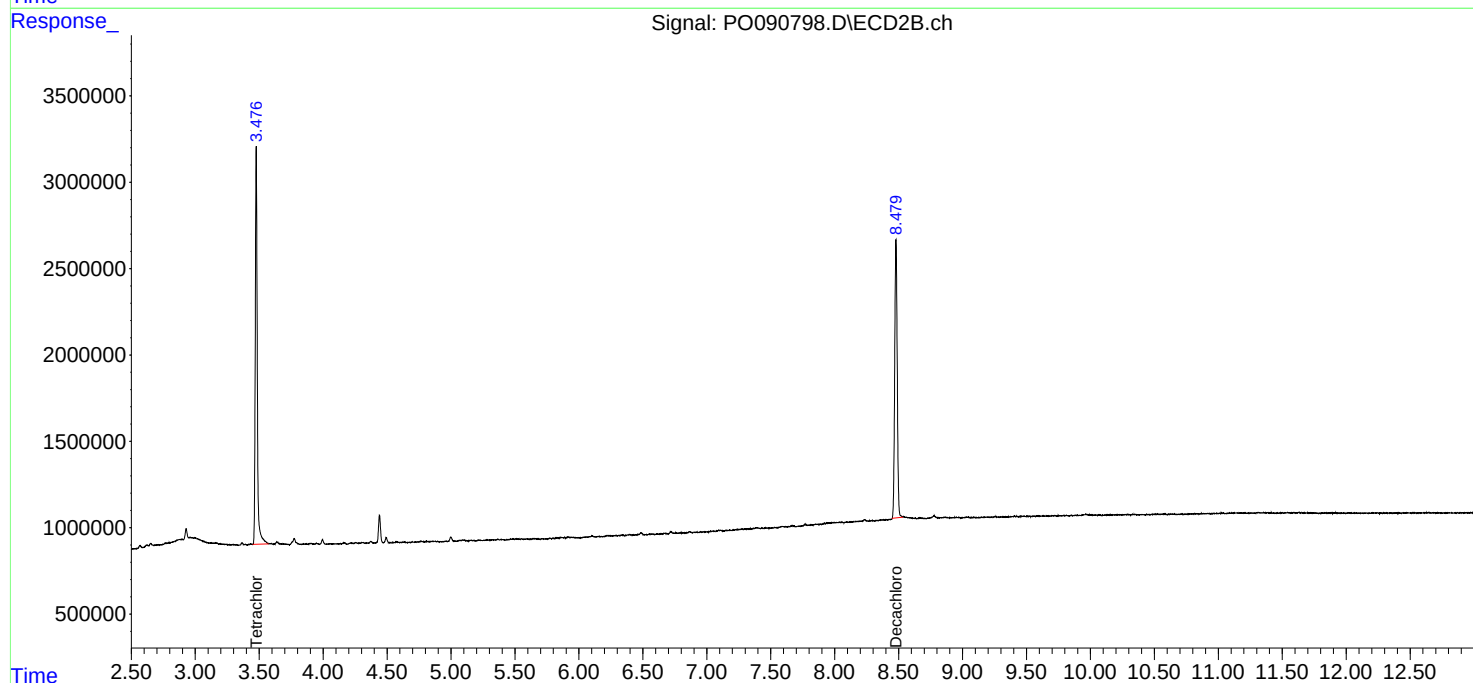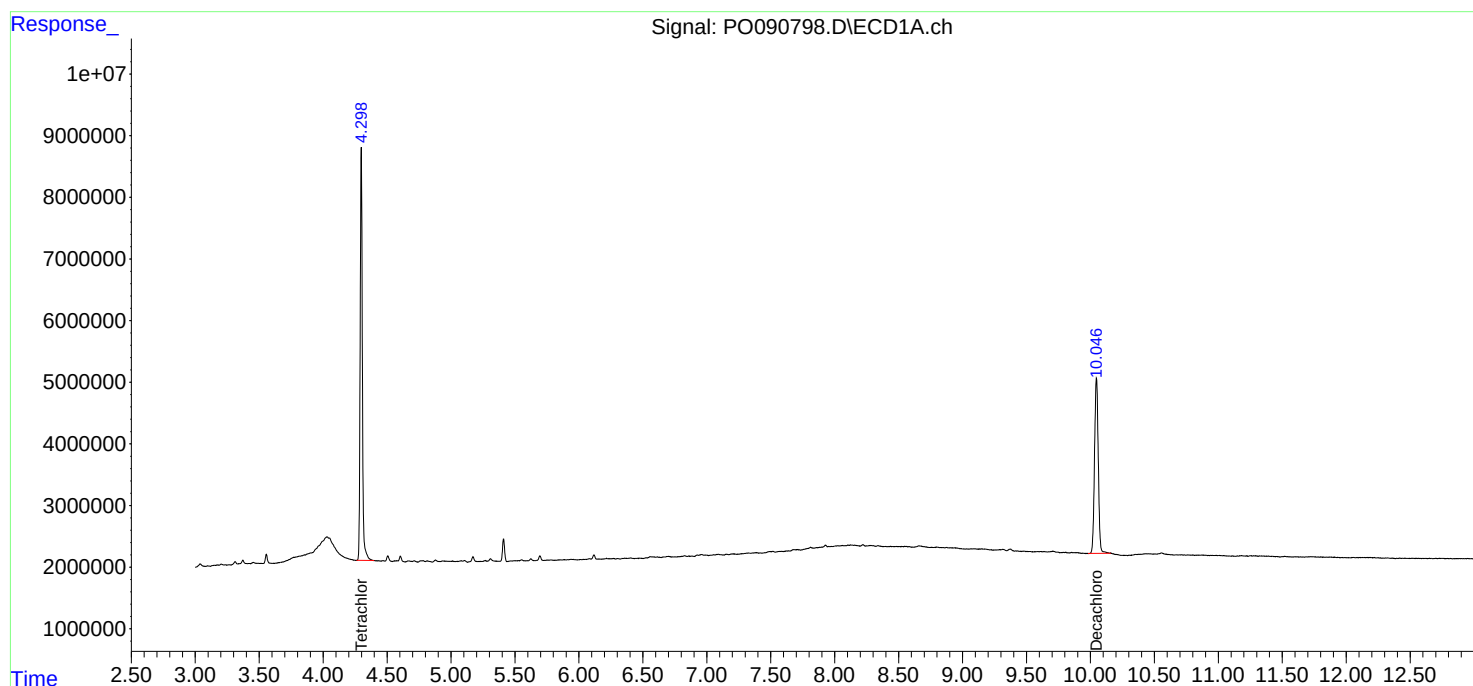


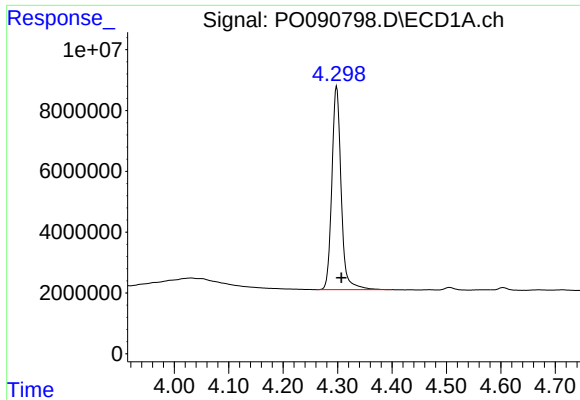

#1 Tetrachloro-m-xylene


R.T.: 4.298 min
Delta R.T.: -0.009 min
Response: 79338837
Conc: 24.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
250FB-BP-BACKFILL-08

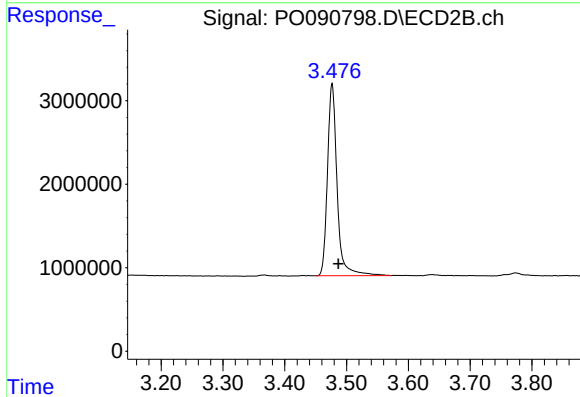


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: -0.010 min
Response: 24998667
Conc: 23.52 ng/ml

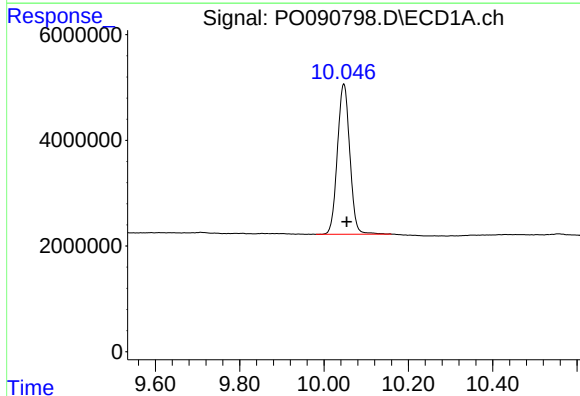

#2 Decachlorobiphenyl

R.T.: 10.047 min
Delta R.T.: -0.007 min
Response: 57913707
Conc: 23.63 ng/ml

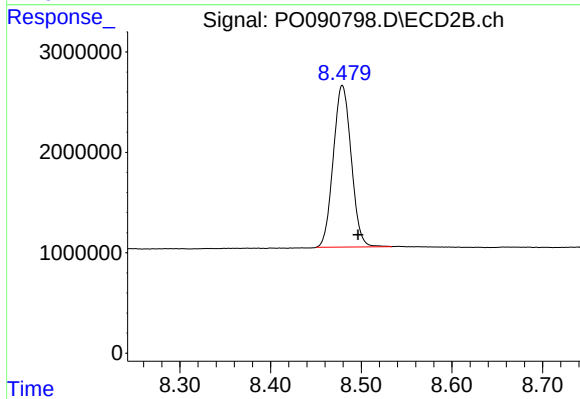

#2 Decachlorobiphenyl

R.T.: 8.479 min
Delta R.T.: -0.017 min
Response: 22116056
Conc: 21.47 ng/ml