

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2024 01:37
 Operator : YP/AJ
 Sample : P4860-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUP-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 03:47:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.371	3.638	188.9E6	71608940	21.695m	21.121
2) SA Decachlor...	10.092	8.633	71633774	72011313	23.454	21.169

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 01:37
Operator : YP/AJ
Sample : P4860-01
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DUP-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 03:47:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

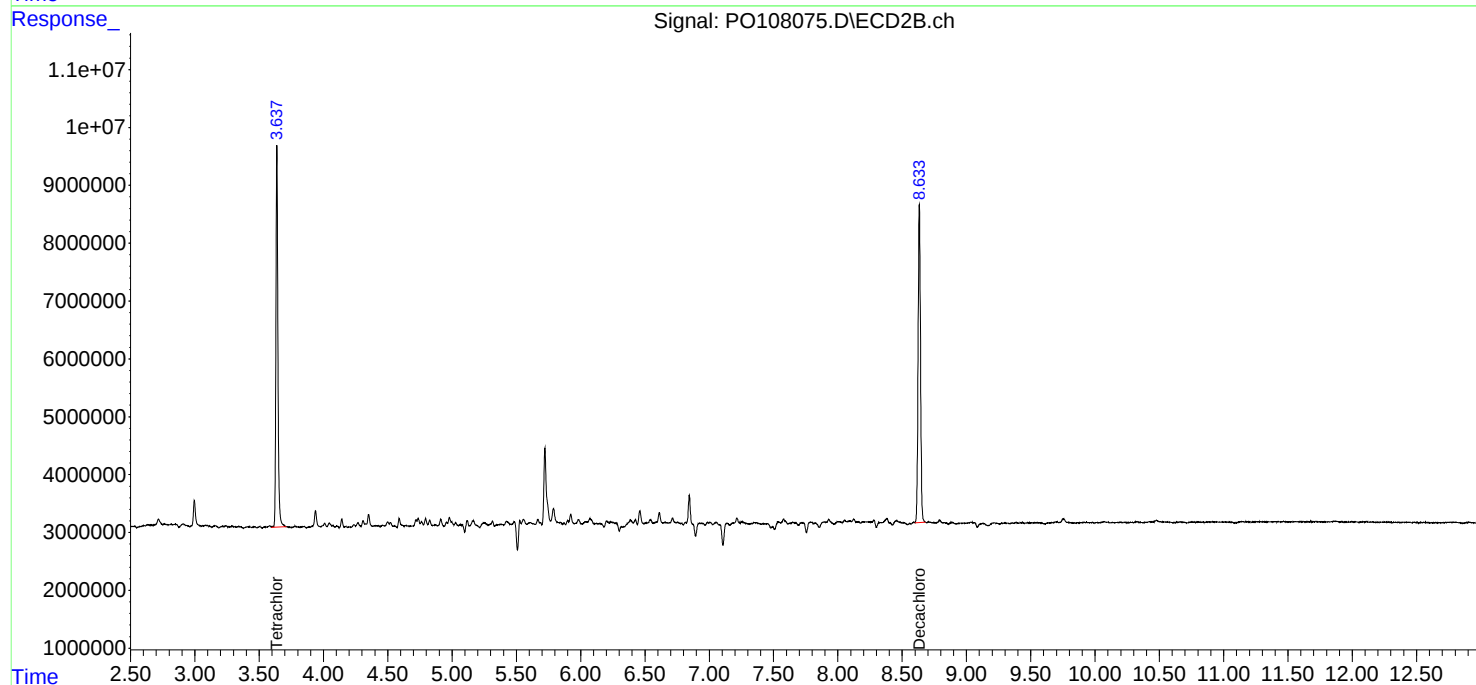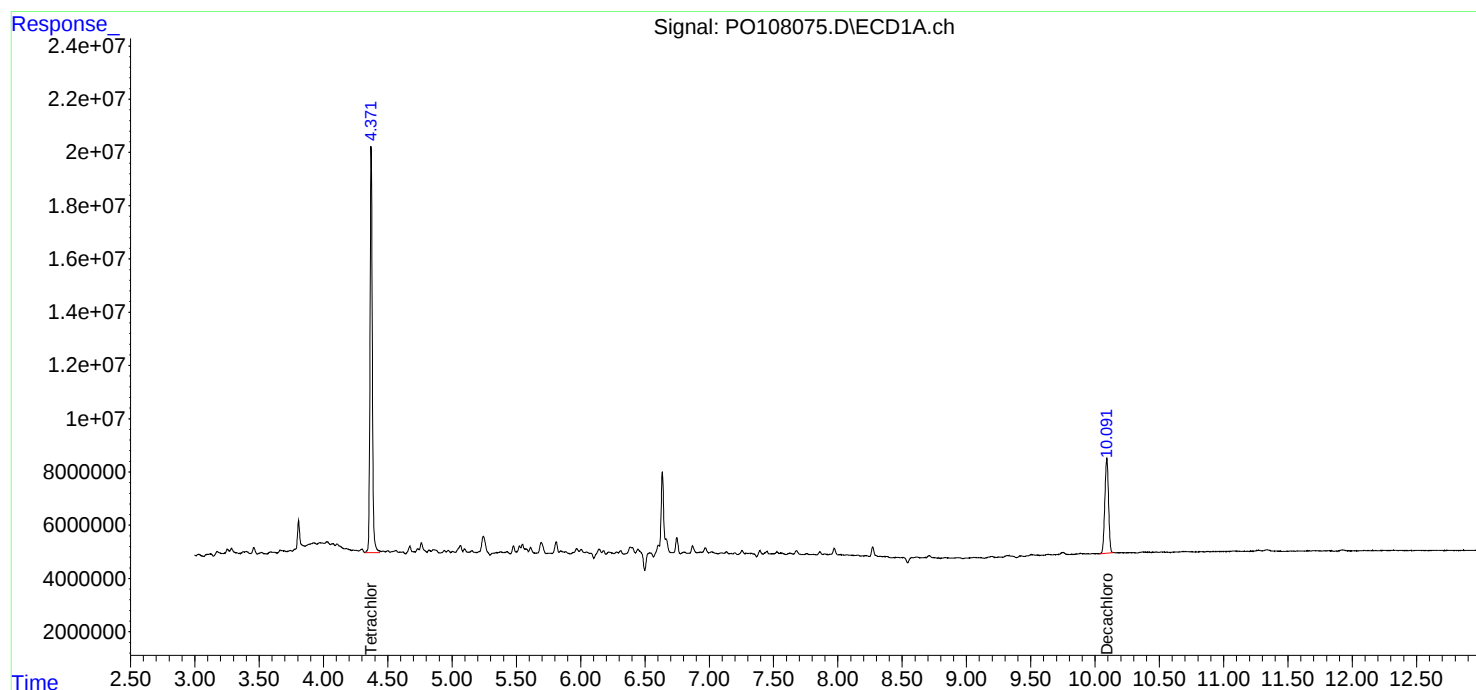

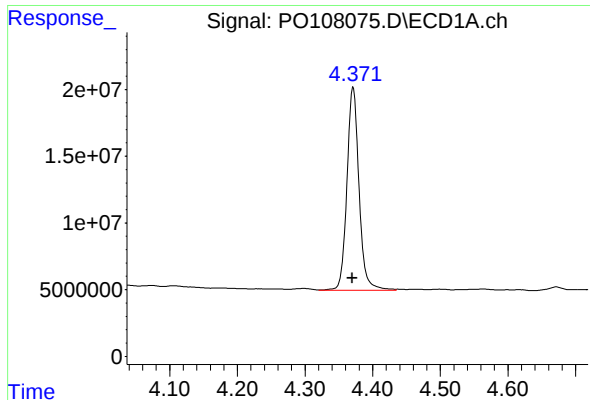


#1 Tetrachloro-m-xylene

R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 188877747
Conc: 21.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

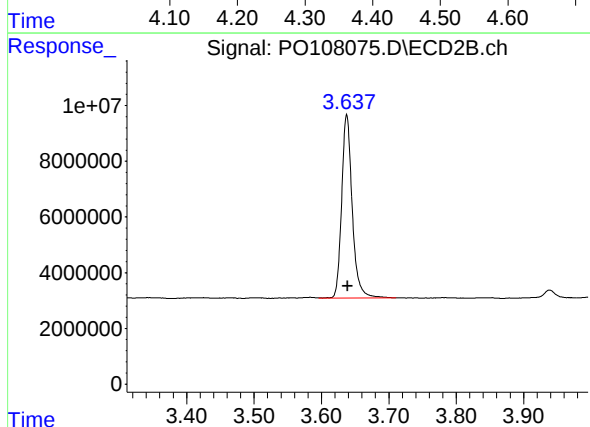


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.001 min
Response: 71608940
Conc: 21.12 ng/ml

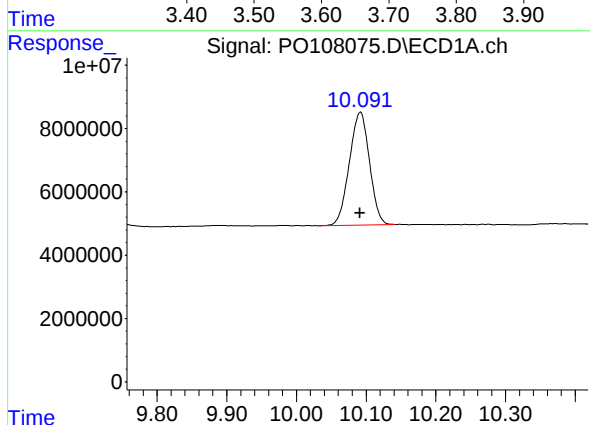

#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: 0.000 min
Response: 71633774
Conc: 23.45 ng/ml

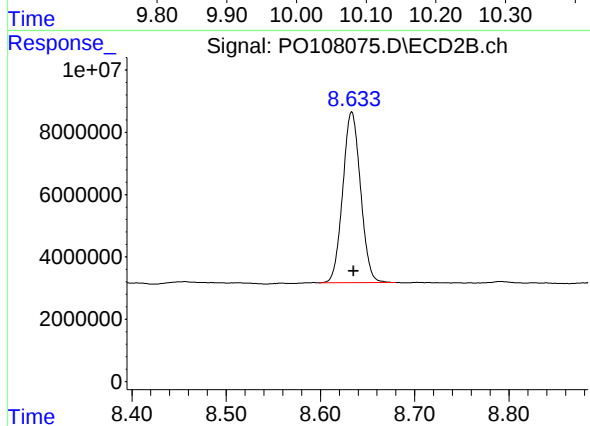

#2 Decachlorobiphenyl

R.T.: 8.633 min
Delta R.T.: -0.002 min
Response: 72011313
Conc: 21.17 ng/ml