

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108079.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2024 02:42
 Operator : YP/AJ
 Sample : P4860-03
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PH2-BOT-002

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 03:48:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.369	3.638	195.9E6	75641144	22.504m	22.310
2) SA Decachlor...	10.089	8.634	73047667	72617205	23.917	21.347

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108079.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 02:42
Operator : YP/AJ
Sample : P4860-03
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PH2-BOT-002


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 03:48:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

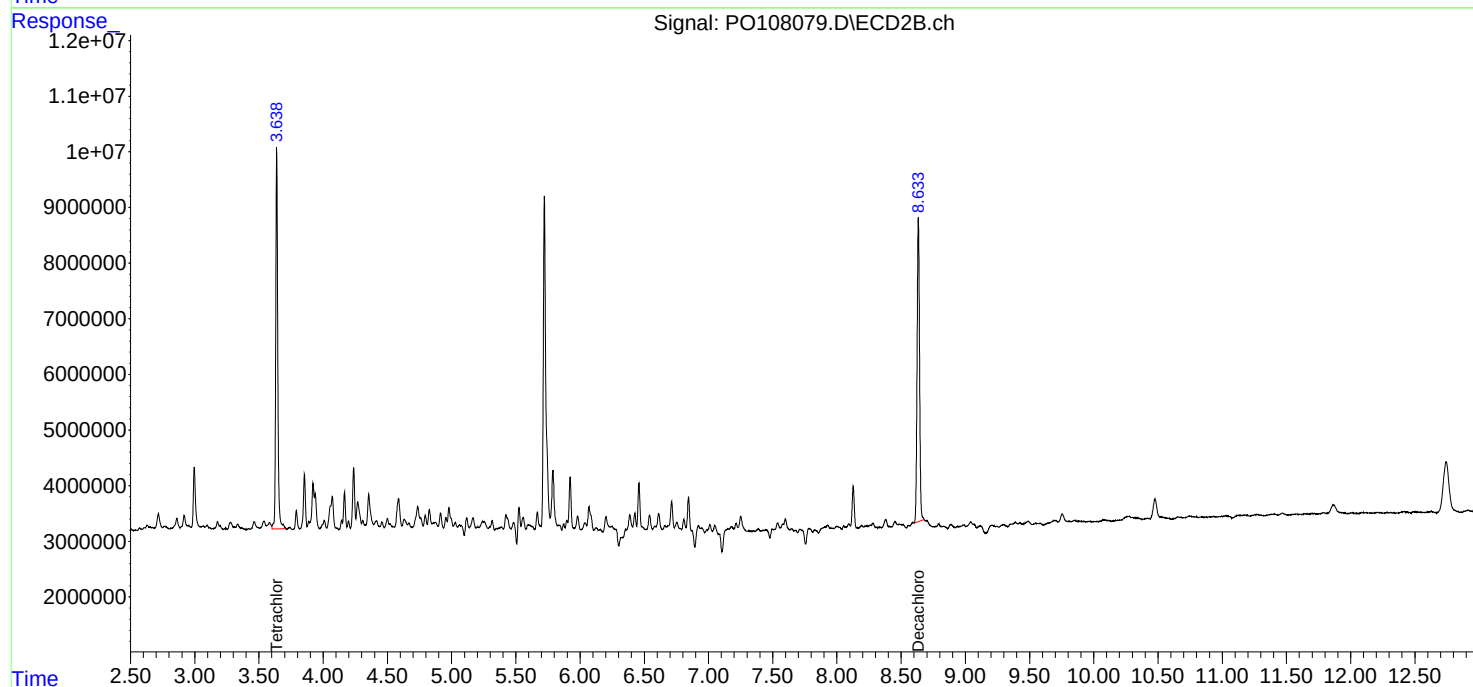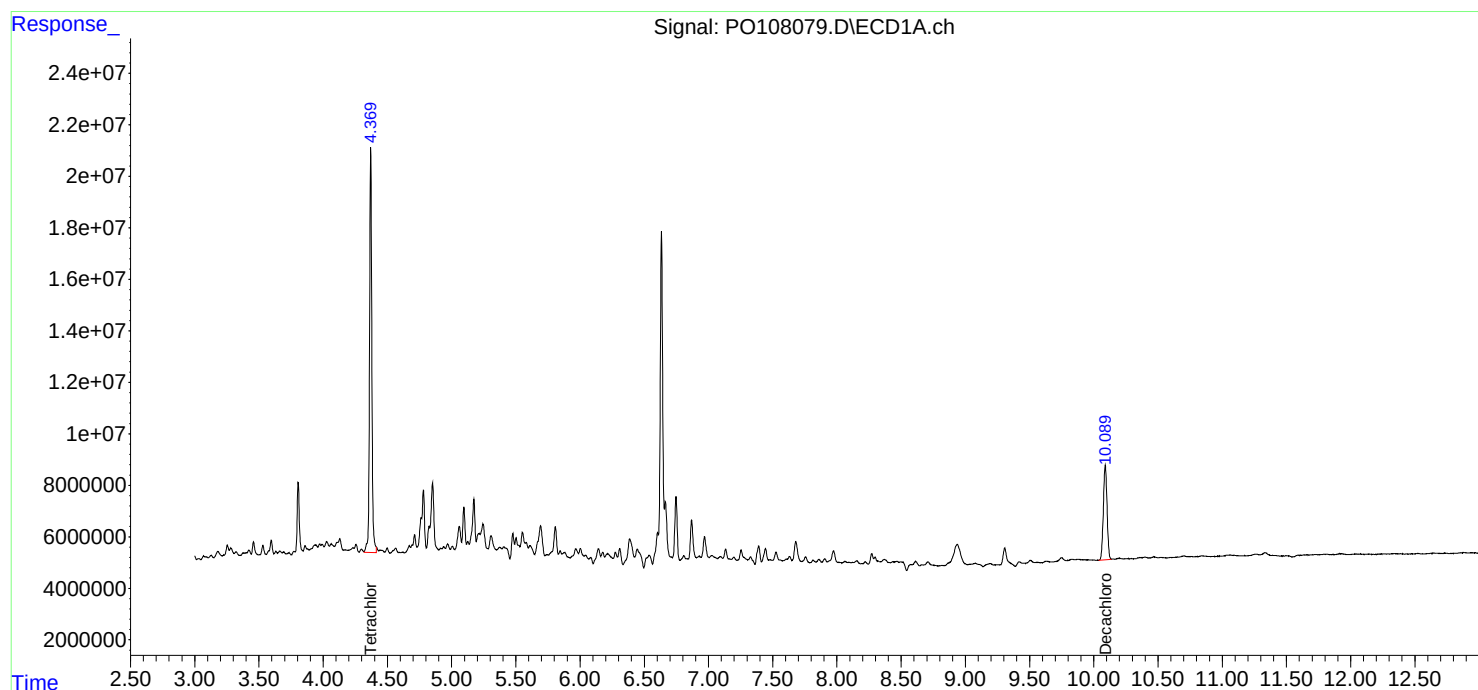

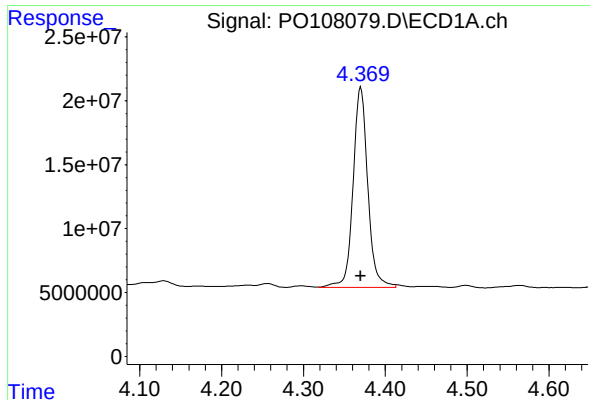


#1 Tetrachloro-m-xylene

R.T.: 4.369 min
Delta R.T.: 0.000 min
Response: 195924166
Conc: 22.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
PH2-BOT-002


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

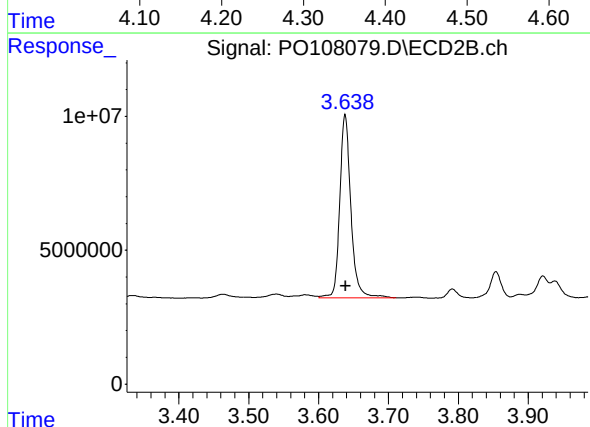


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: 0.000 min
Response: 75641144
Conc: 22.31 ng/ml

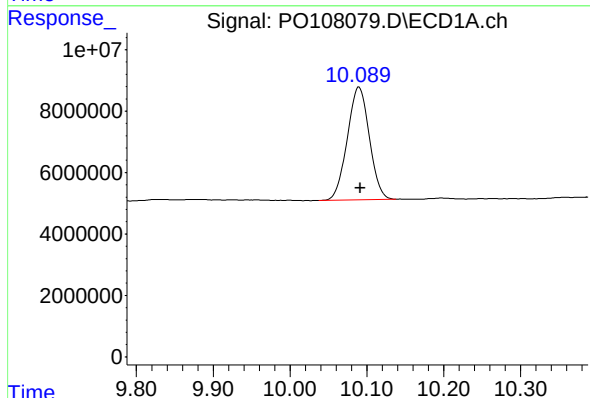

#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: -0.002 min
Response: 73047667
Conc: 23.92 ng/ml

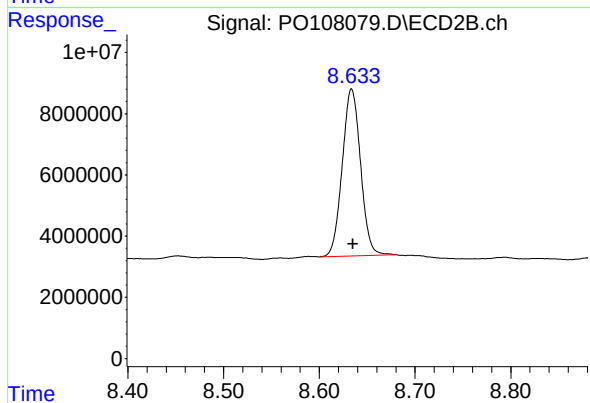

#2 Decachlorobiphenyl

R.T.: 8.634 min
Delta R.T.: -0.002 min
Response: 72617205
Conc: 21.35 ng/ml