

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111919\
 Data File : P0063877.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2019 12:48
 Operator : SM/AJ
 Sample : K5904-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 14:45:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.568	601819	440748	19.683	19.843
2)	SA Decachlor...	9.943	8.538	841923	710781	20.719	24.303
Target Compounds							
9)	L2 AR-1221-2	4.619	3.866	8973	7122	28.607	33.873
10)	L2 AR-1221-3	4.619	0.000	8973	0	9.460	N.D. #
11)	L3 AR-1232-1	4.619	0.000	8973	0	6.746	N.D. #
33)	L7 AR-1260-3	0.000	6.517	0	4347	N.D.	2.437 #
39)	L8 AR-1262-4	0.000	7.561	0	32794	N.D.	9.289 #
42)	L9 AR-1268-2	0.000	7.561	0	32794	N.D.	6.581 #
43)	L9 AR-1268-3	0.000	7.724	0	5307	N.D.	1.337 #
45)	L9 AR-1268-5	0.000	8.291	0	8656	N.D.	0.732 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111919\
Data File : P0063877.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2019 12:48
Operator : SM/AJ
Sample : K5904-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 14:45:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

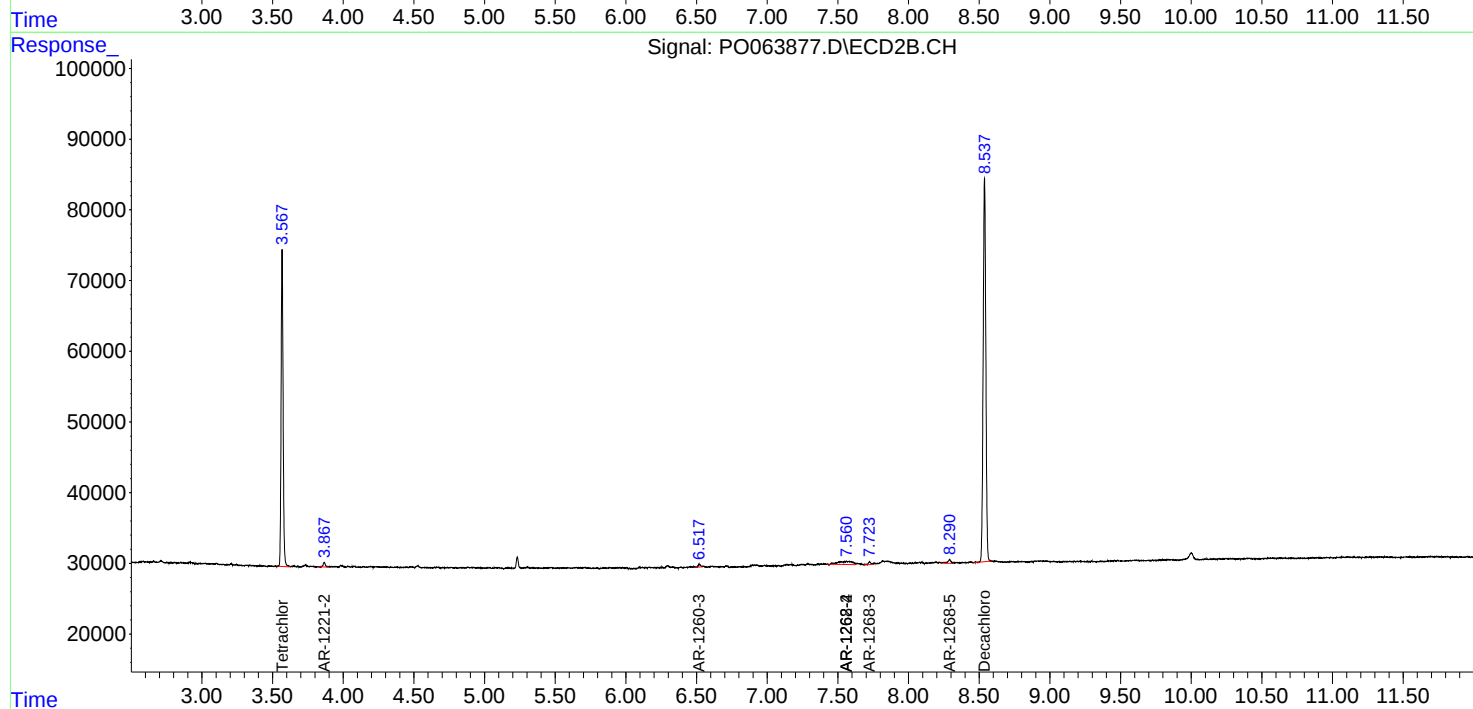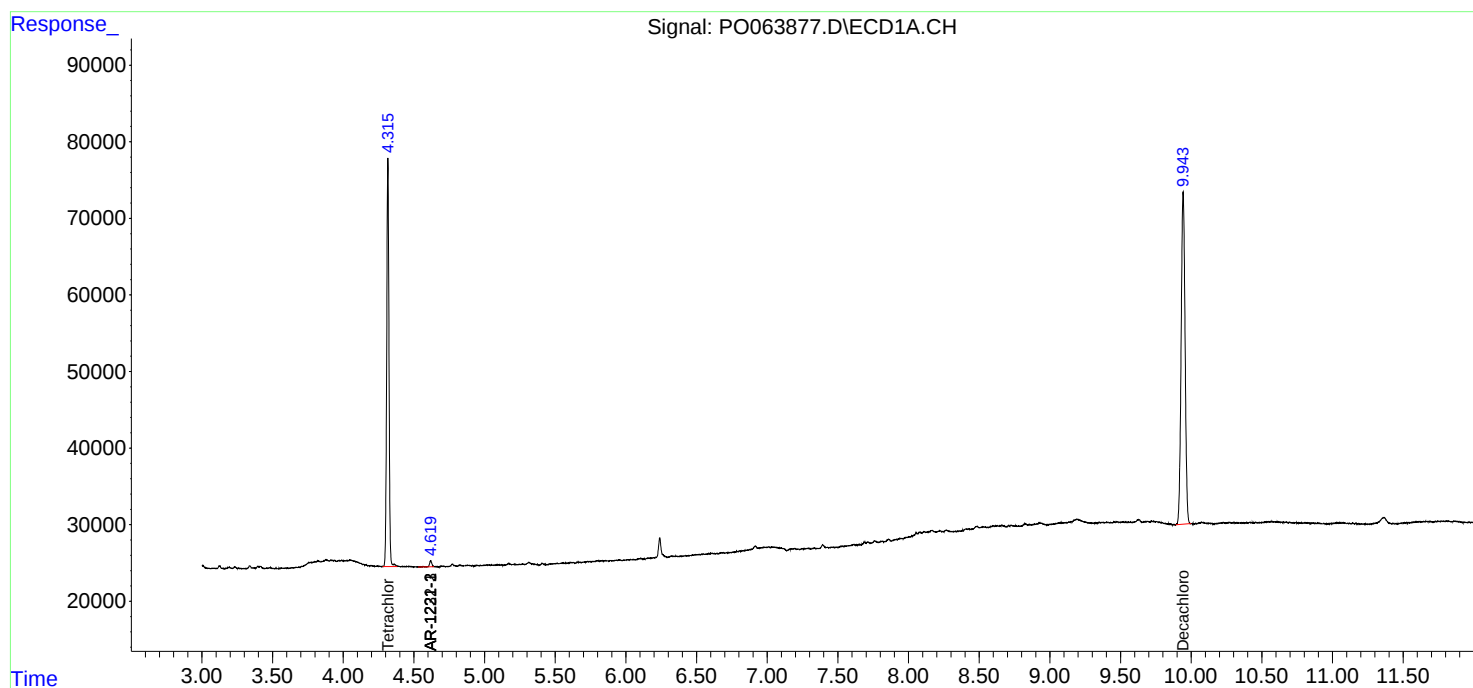


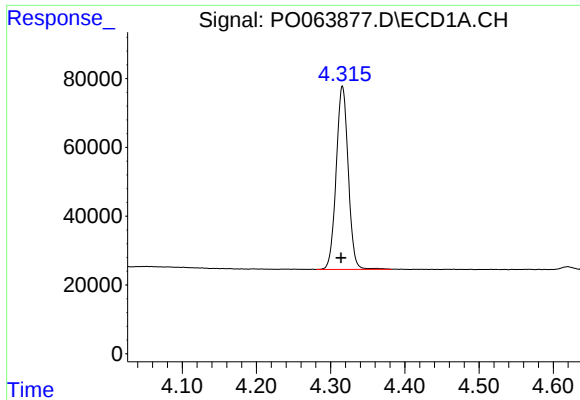

#1 Tetrachloro-m-xylene


R.T.: 4.316 min
Delta R.T.: 0.002 min
Response: 601819
Conc: 19.68 ng/ml

Instrument :
ECD_O
ClientSampleId :

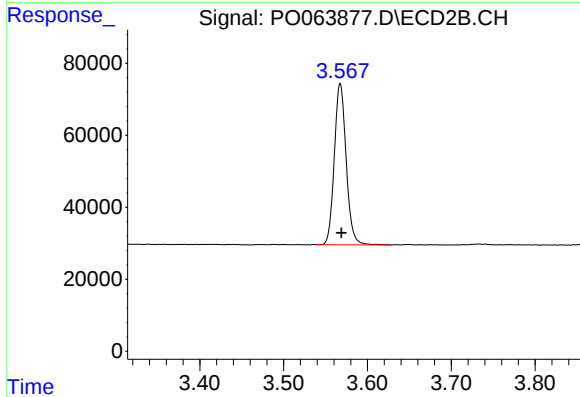


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: -0.001 min
Response: 440748
Conc: 19.84 ng/ml

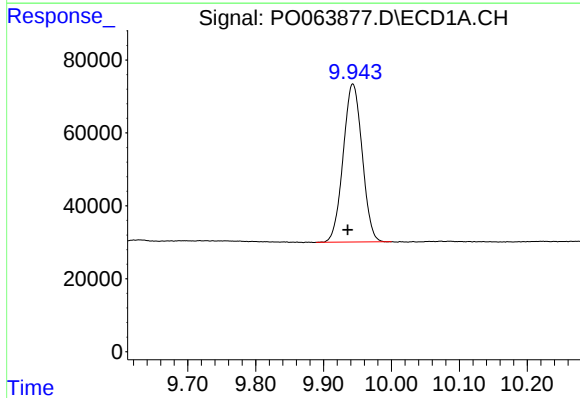


#2 Decachlorobiphenyl

R.T.: 9.943 min
Delta R.T.: 0.007 min
Response: 841923
Conc: 20.72 ng/ml

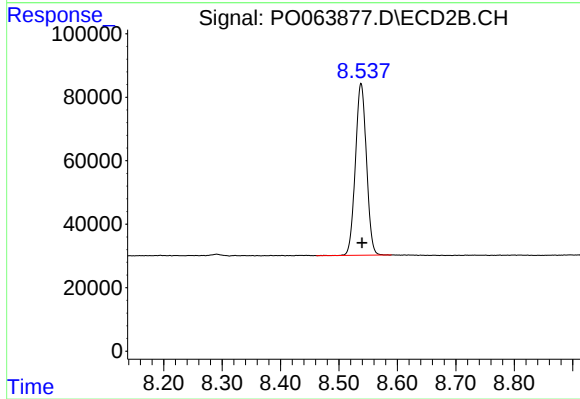

#2 Decachlorobiphenyl


R.T.: 8.538 min
Delta R.T.: -0.002 min
Response: 710781
Conc: 24.30 ng/ml

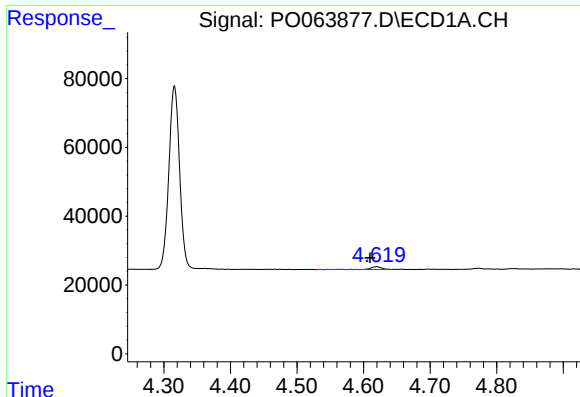

#9 AR-1221-2


R.T.: 4.619 min
Delta R.T.: 0.010 min
Response: 8973
Conc: 28.61 ng/ml

Instrument :
ECD_O
ClientSampleId :

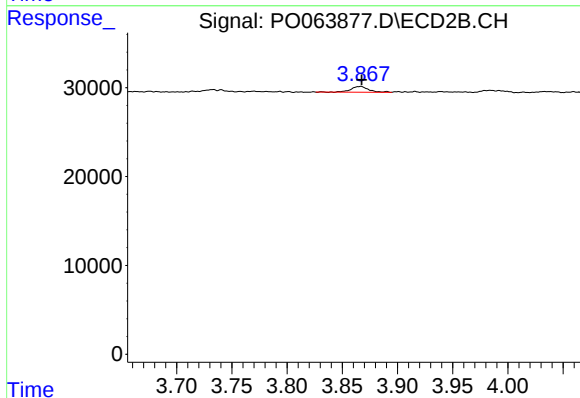


#9 AR-1221-2

R.T.: 3.866 min
Delta R.T.: -0.001 min
Response: 7122
Conc: 33.87 ng/ml

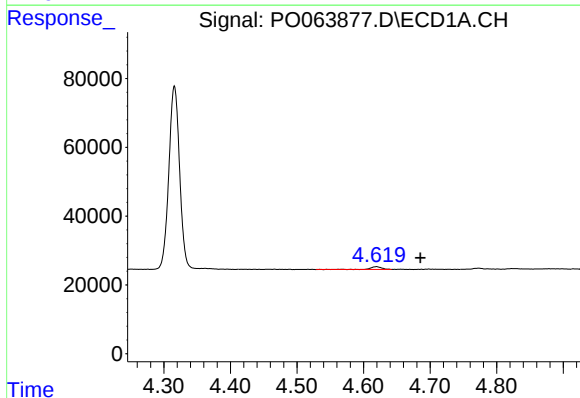


#10 AR-1221-3

R.T.: 4.619 min
Delta R.T.: -0.066 min
Response: 8973
Conc: 9.46 ng/ml

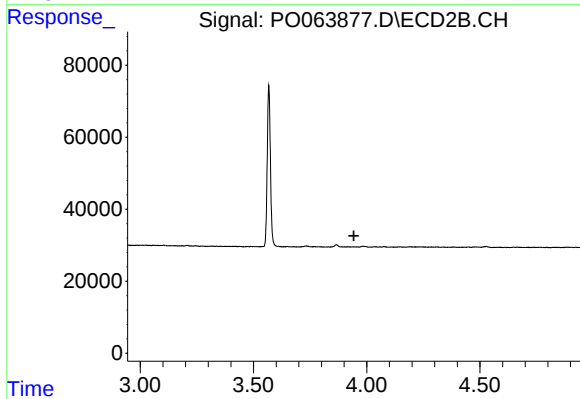

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 3.944 min
Response: 0
Conc: N.D.

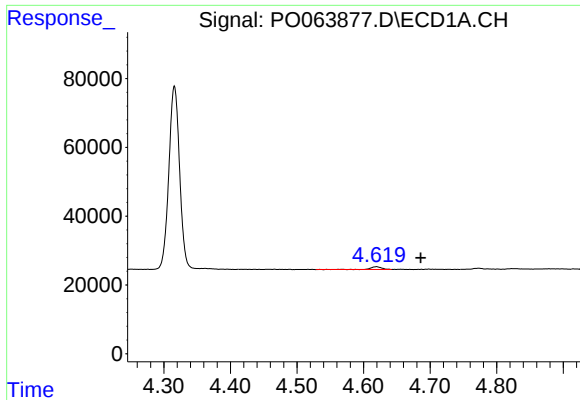

#11 AR-1232-1


R.T.: 4.619 min
Delta R.T.: -0.066 min
Response: 8973
Conc: 6.75 ng/ml

Instrument :
ECD_O
ClientSampleId :

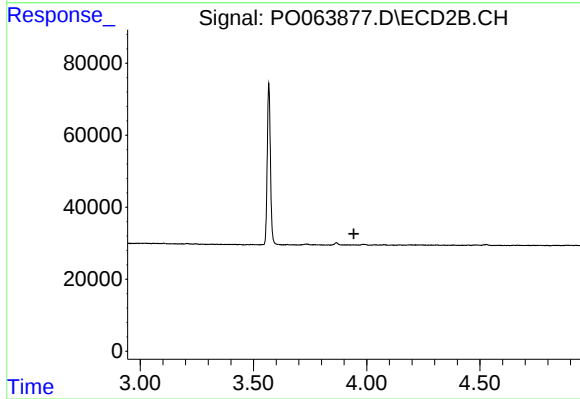


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.943 min
Response: 0
Conc: N.D.

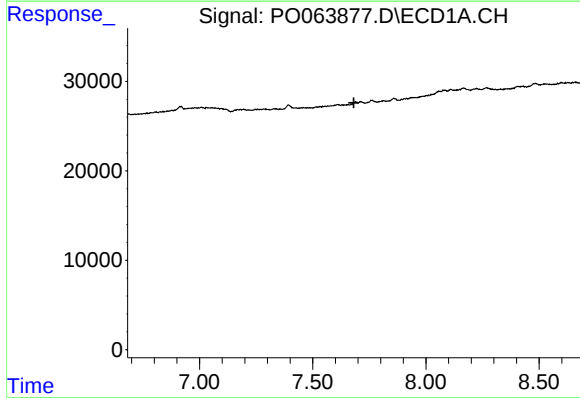


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.682 min
Response: 0
Conc: N.D.

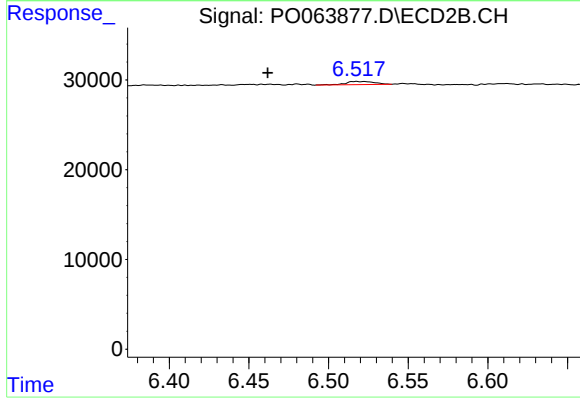

#33 AR-1260-3


R.T.: 6.517 min
Delta R.T.: 0.056 min
Response: 4347
Conc: 2.44 ng/ml

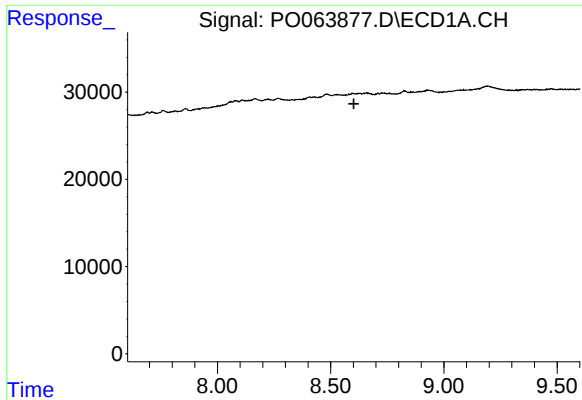

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

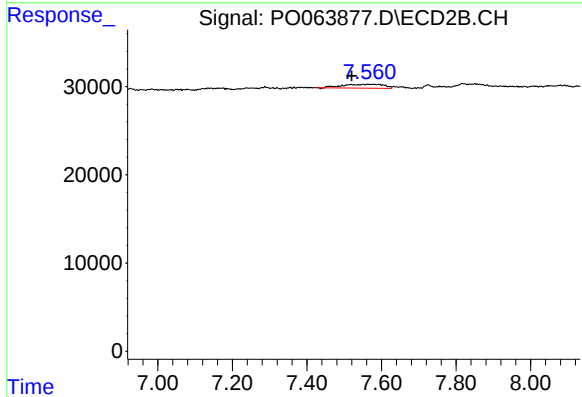


#39 AR-1262-4

R.T.: 7.561 min
Delta R.T.: 0.042 min
Response: 32794
Conc: 9.29 ng/ml

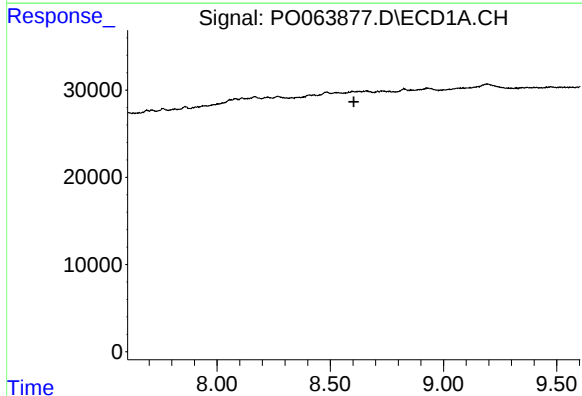


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.604 min
Response: 0
Conc: N.D.

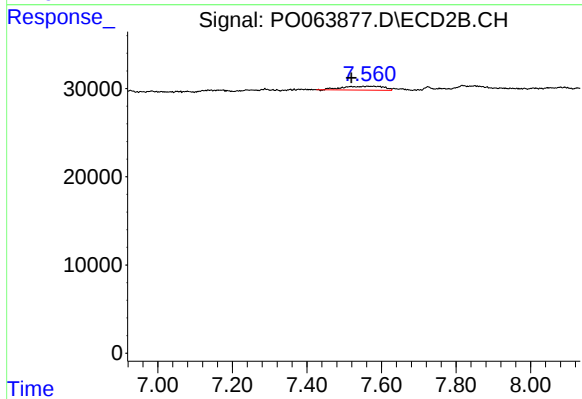

#42 AR-1268-2

R.T.: 7.561 min
Delta R.T.: 0.042 min
Response: 32794
Conc: 6.58 ng/ml

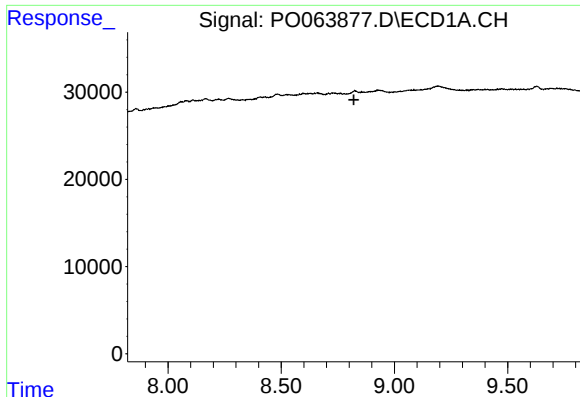

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

#43 AR-1268-3

R.T.: 7.724 min
Delta R.T.: -0.003 min
Response: 5307
Conc: 1.34 ng/ml

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.619 min
Response: 0
Conc: N.D.

#45 AR-1268-5

R.T.: 8.291 min
Delta R.T.: -0.002 min
Response: 8656
Conc: 0.73 ng/ml