

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111919\
 Data File : P0063887.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2019 15:50
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 03:59:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.568	480677	353592	15.721	15.919
2)	SA Decachlor...	9.944	8.537	693416	577320	17.065	19.740
Target Compounds							
7)	L1 AR-1016-5	0.000	5.157	0	5025	N.D.	6.326 #
9)	L2 AR-1221-2	0.000	3.866	0	5030	N.D.	23.921 #
15)	L3 AR-1232-5	0.000	5.157	0	5025	N.D.	9.747 #
24)	L5 AR-1248-4	0.000	5.157	0	5025	N.D.	4.667 #
32)	L7 AR-1260-2	7.393	0.000	6631	0	2.632	N.D. #
43)	L9 AR-1268-3	0.000	7.726	0	4056	N.D.	1.022 #
45)	L9 AR-1268-5	0.000	8.292	0	8098	N.D.	0.685 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111919\
Data File : PO063887.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2019 15:50
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 03:59:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

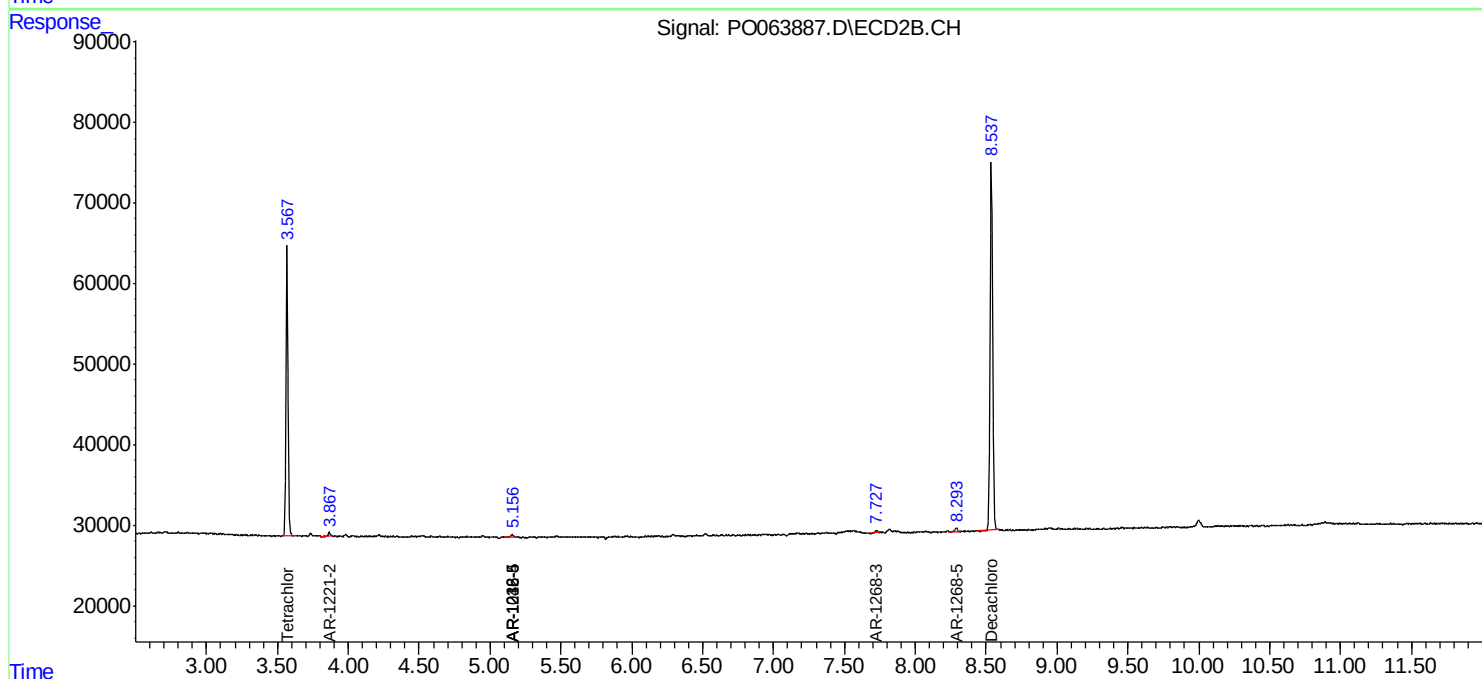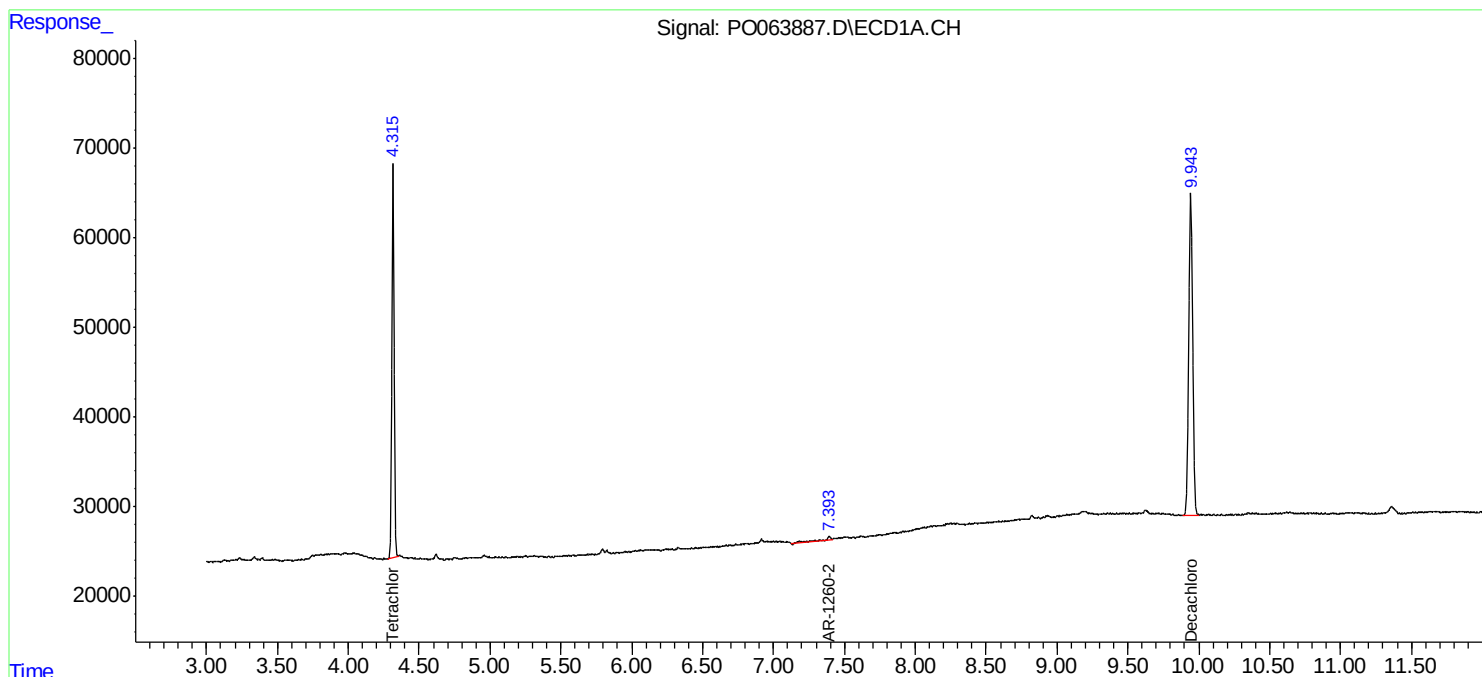


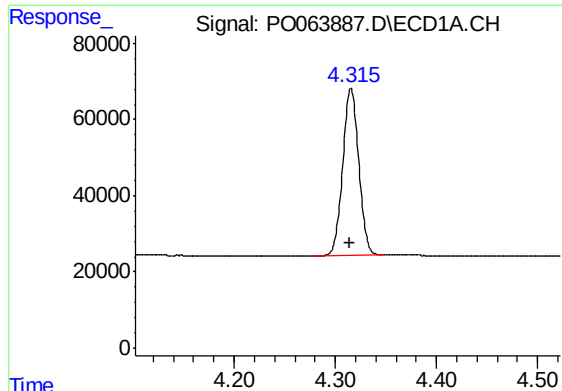

#1 Tetrachloro-m-xylene


R.T.: 4.316 min
Delta R.T.: 0.002 min
Response: 480677
Conc: 15.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

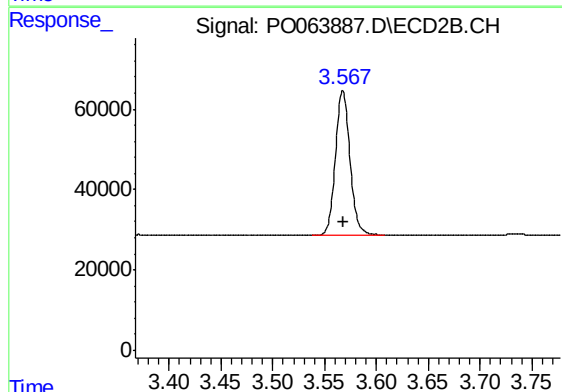


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: -0.001 min
Response: 353592
Conc: 15.92 ng/ml

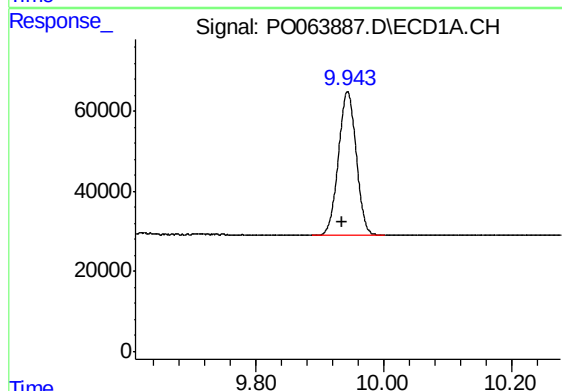


#2 Decachlorobiphenyl

R.T.: 9.944 min
Delta R.T.: 0.008 min
Response: 693416
Conc: 17.06 ng/ml

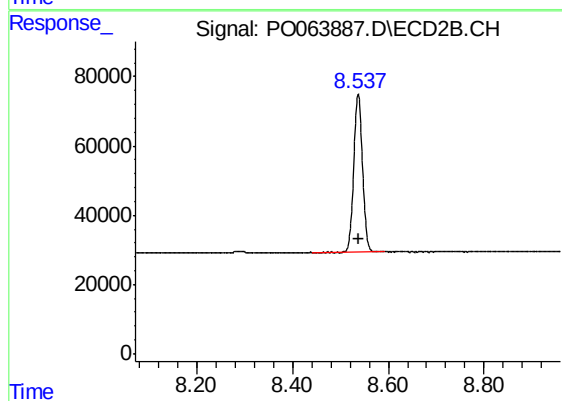

#2 Decachlorobiphenyl


R.T.: 8.537 min
Delta R.T.: -0.002 min
Response: 577320
Conc: 19.74 ng/ml

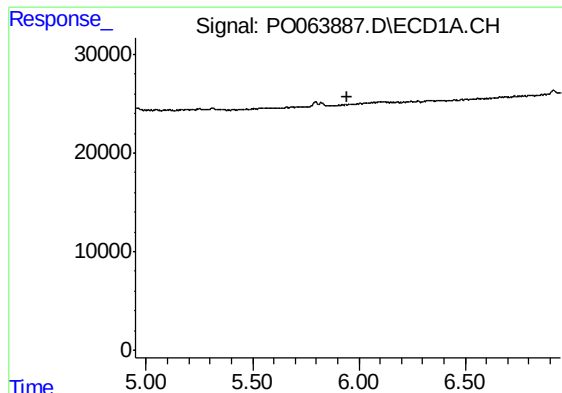

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

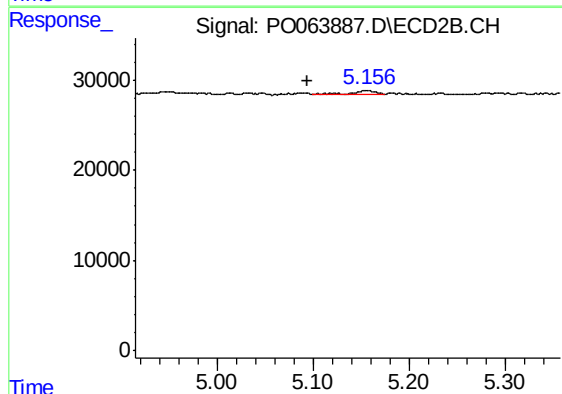


#7 AR-1016-5

R.T.: 5.157 min
Delta R.T.: 0.063 min
Response: 5025
Conc: 6.33 ng/ml

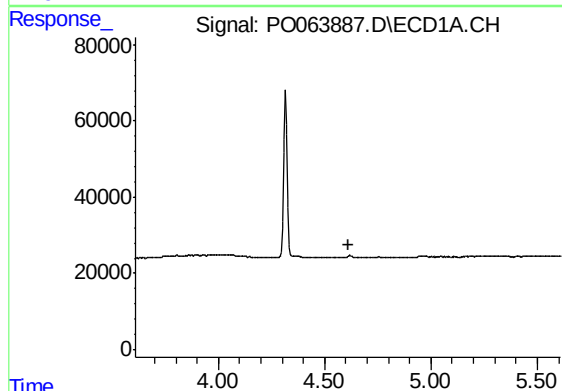


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.610 min
Response: 0
Conc: N.D.

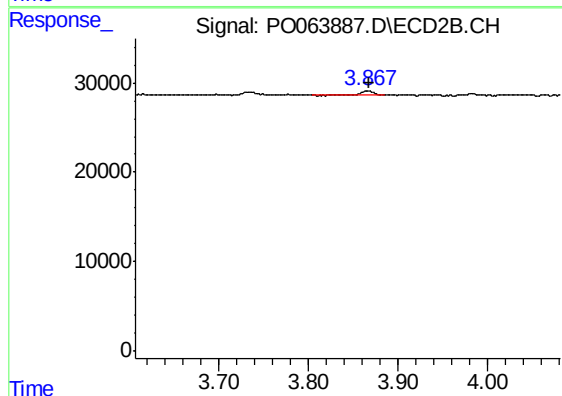

#9 AR-1221-2


R.T.: 3.866 min
Delta R.T.: -0.001 min
Response: 5030
Conc: 23.92 ng/ml

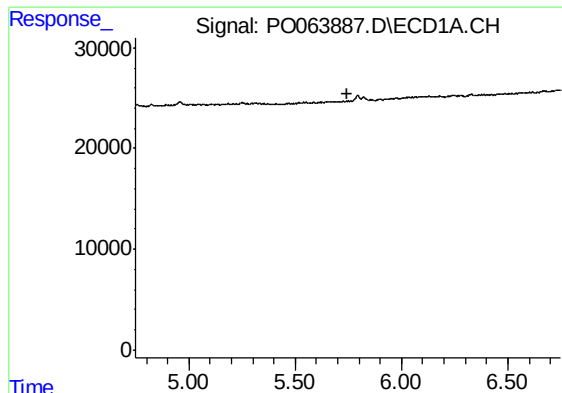

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.748 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

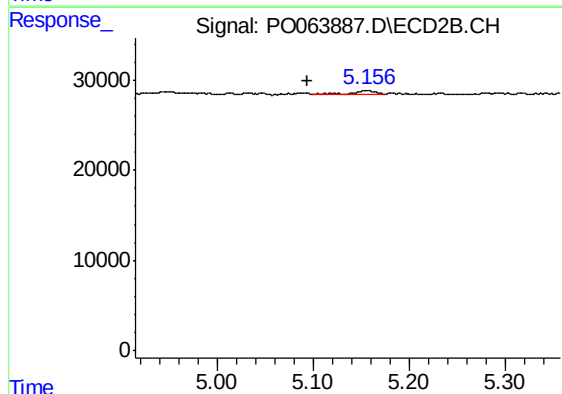


#15 AR-1232-5

R.T.: 5.157 min
Delta R.T.: 0.062 min
Response: 5025
Conc: 9.75 ng/ml

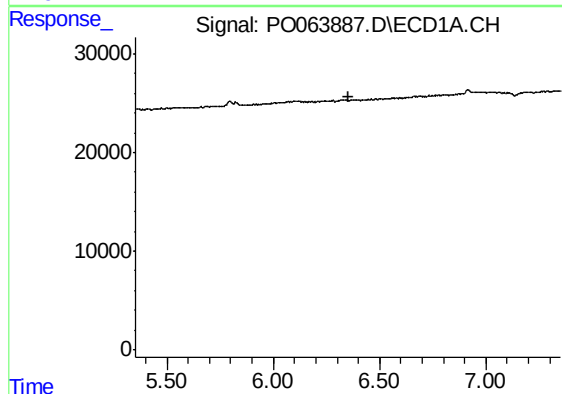


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.351 min
Response: 0
Conc: N.D.

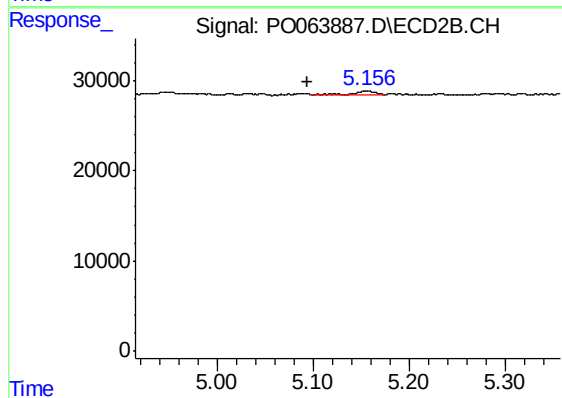

#24 AR-1248-4


R.T.: 5.157 min
Delta R.T.: 0.062 min
Response: 5025
Conc: 4.67 ng/ml

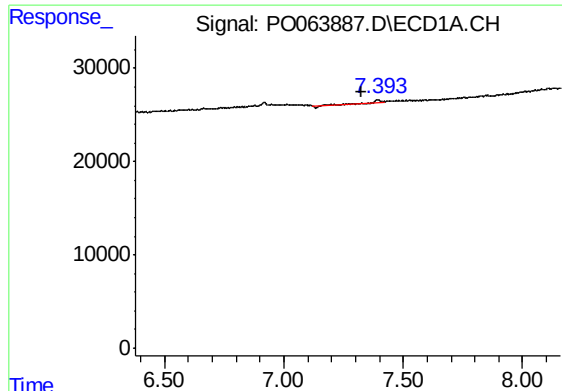

#32 AR-1260-2


R.T.: 7.393 min
Delta R.T.: 0.068 min
Response: 6631
Conc: 2.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

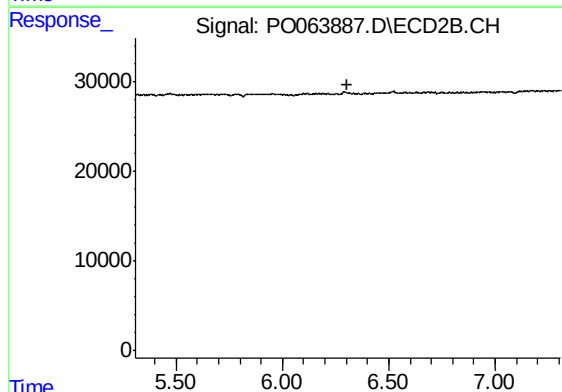


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.308 min
Response: 0
Conc: N.D.

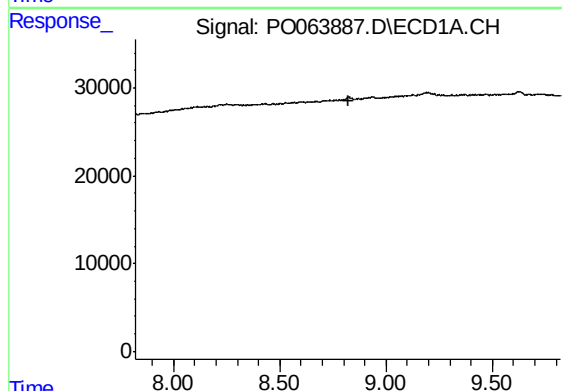


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

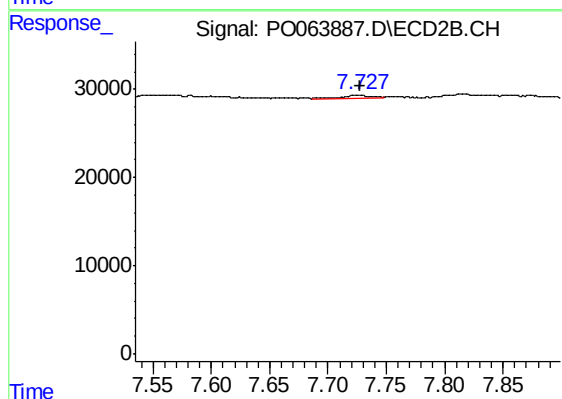

#43 AR-1268-3


R.T.: 7.726 min
Delta R.T.: -0.001 min
Response: 4056
Conc: 1.02 ng/ml

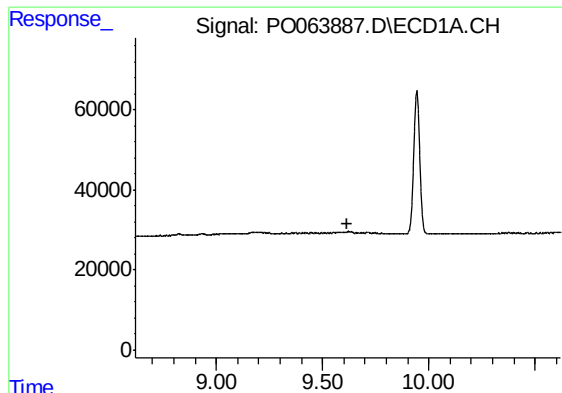

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.619 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

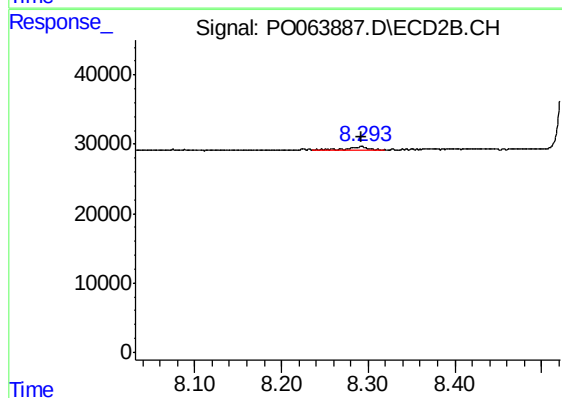

#45 AR-1268-5

R.T.: 8.292 min
Delta R.T.: 0.000 min
Response: 8098
Conc: 0.68 ng/ml