

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111920\
 Data File : PO073362.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2020 21:51
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 03:25:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 19 12:09:14 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.942	4.011	1289522	782300	20.493	21.792
2) SA Decachlor...	10.966	9.282	1200661	730129	22.432	20.898

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111920\
Data File : PO073362.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2020 21:51
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 03:25:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 19 12:09:14 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

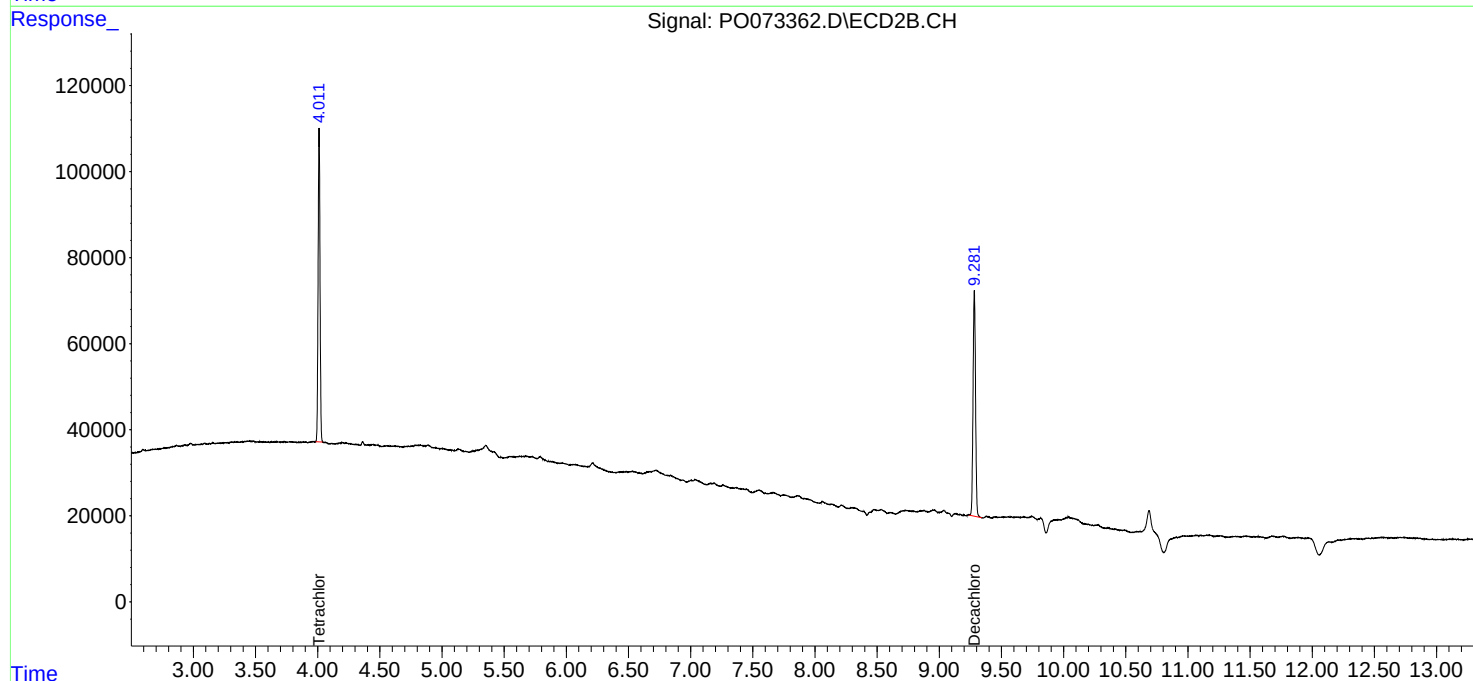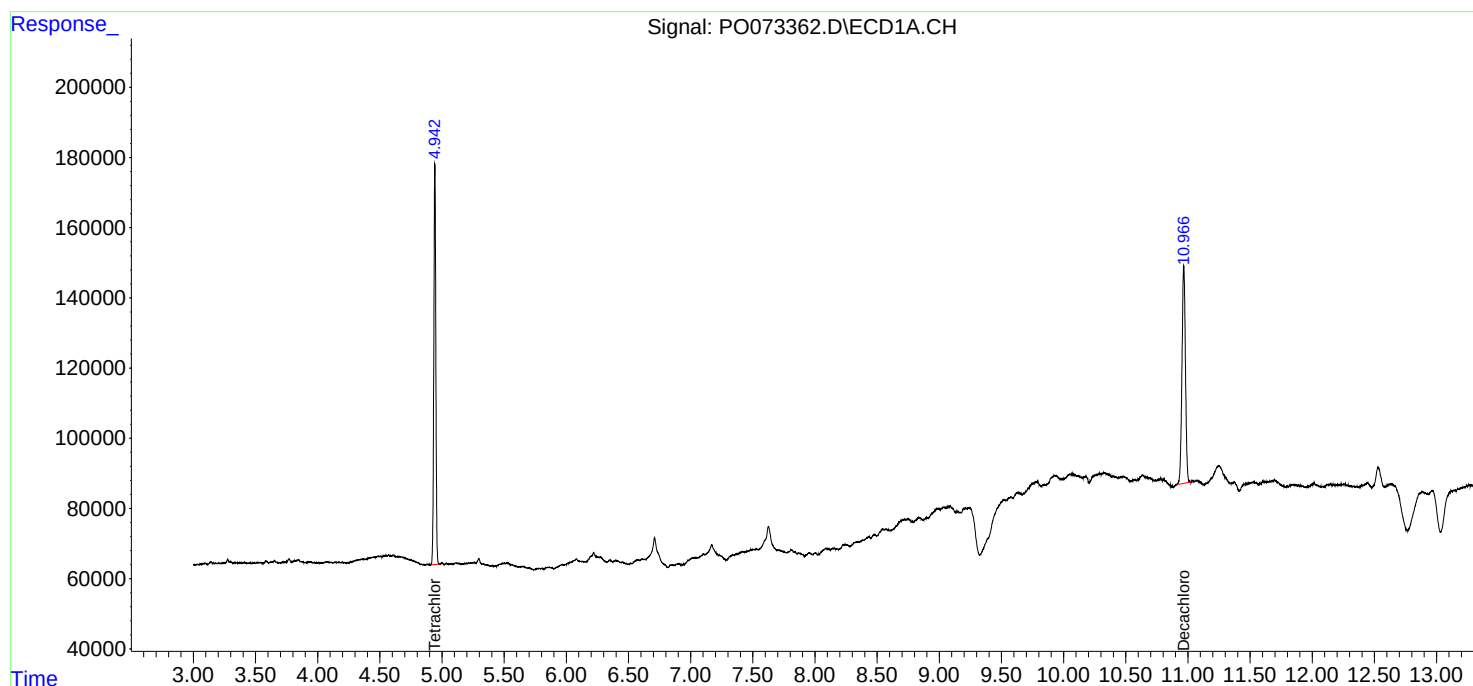


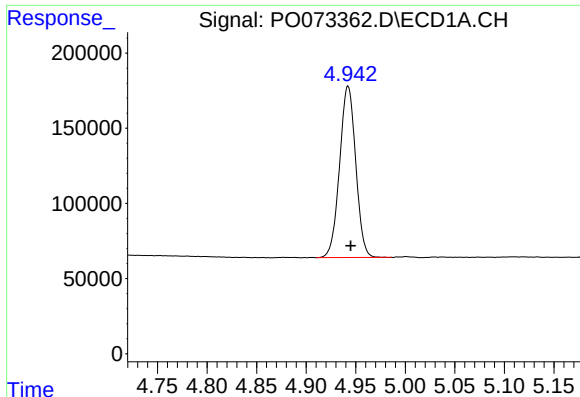

#1 Tetrachloro-m-xylene


R.T.: 4.942 min
Delta R.T.: -0.003 min
Response: 1289522
Conc: 20.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

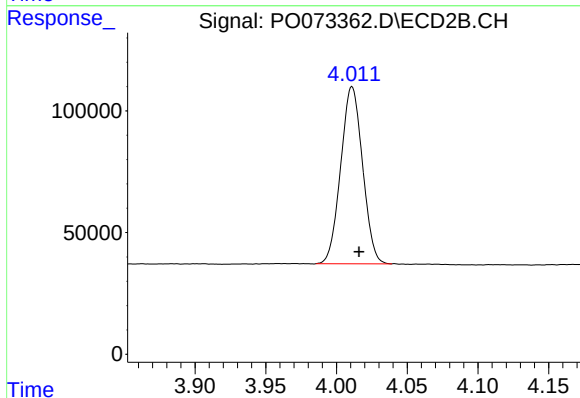


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.005 min
Response: 782300
Conc: 21.79 ng/ml

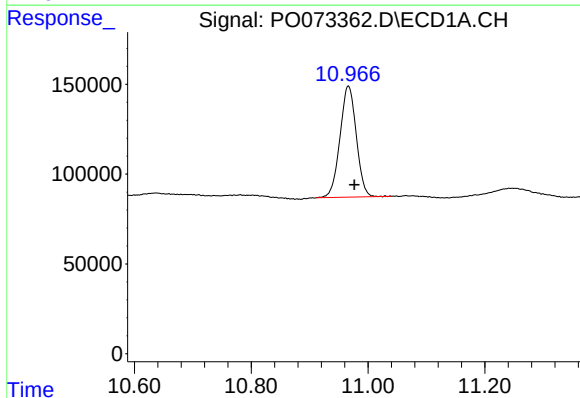

#2 Decachlorobiphenyl

R.T.: 10.966 min
Delta R.T.: -0.010 min
Response: 1200661
Conc: 22.43 ng/ml

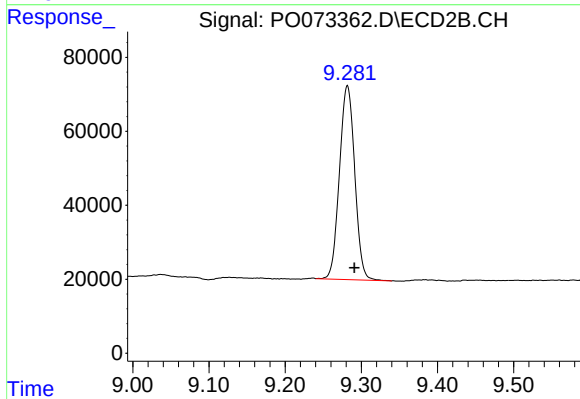

#2 Decachlorobiphenyl

R.T.: 9.282 min
Delta R.T.: -0.009 min
Response: 730129
Conc: 20.90 ng/ml