

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111924\
 Data File : P0108097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2024 14:40
 Operator : YP/AJ
 Sample : P4892-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WB-310-TOP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2024
 Supervised By :Ankita Jodhani 11/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 03:12:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.369	3.638	125.3E6	49854878	14.391m	14.705
2) SA Decachlor...	10.091	8.633	45187961	41123449	14.795	12.089m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111924\
Data File : PO108097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 14:40
Operator : YP/AJ
Sample : P4892-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WB-310-TOP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :Ankita Jodhani 11/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 03:12:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

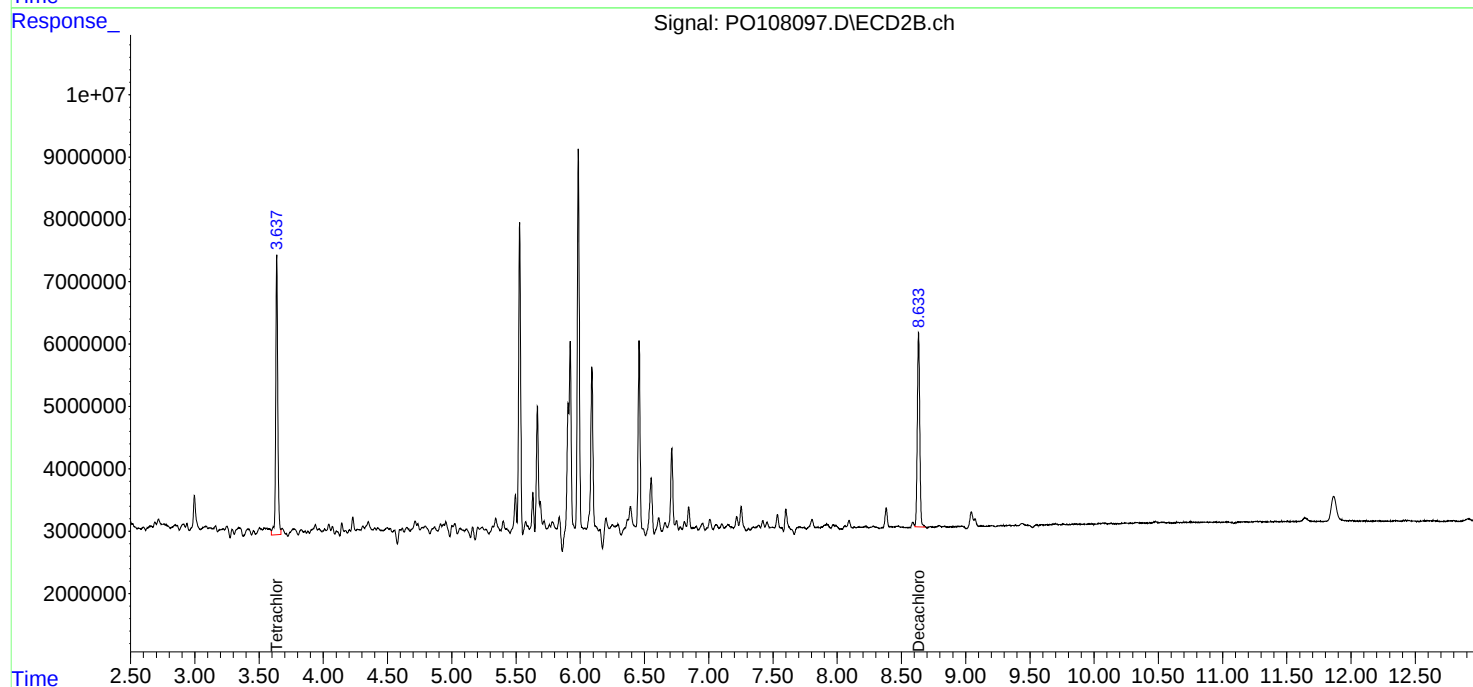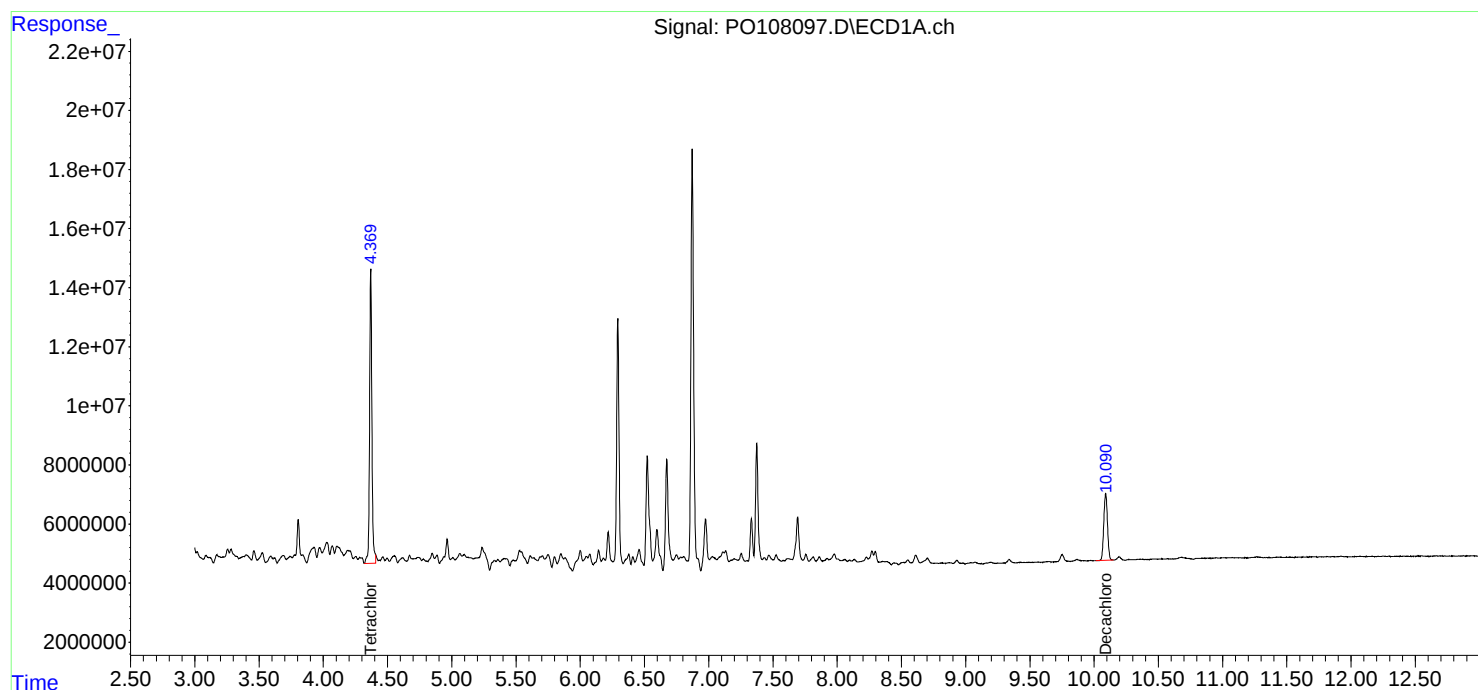

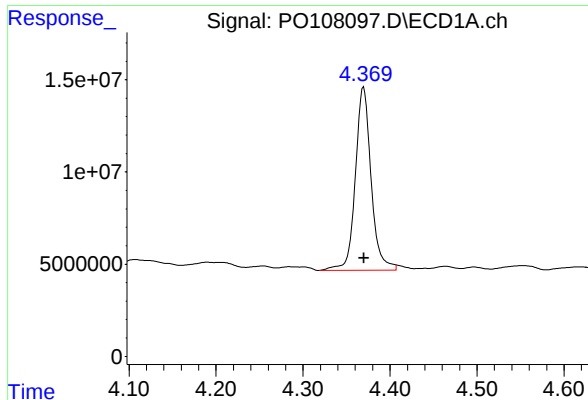


#1 Tetrachloro-m-xylene

R.T.: 4.369 min
Delta R.T.: -0.001 min
Response: 125293430
Conc: 14.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
WB-310-TOP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2024
Supervised By :Ankita Jodhani 11/20/2024

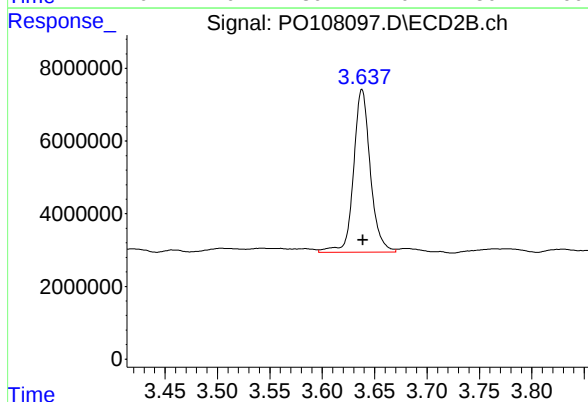


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: 0.000 min
Response: 49854878
Conc: 14.70 ng/ml

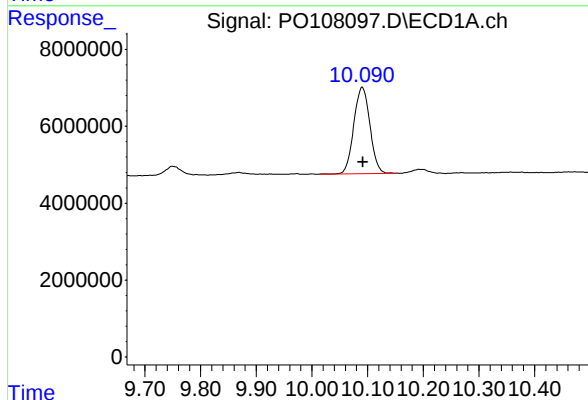

#2 Decachlorobiphenyl

R.T.: 10.091 min
Delta R.T.: 0.000 min
Response: 45187961
Conc: 14.80 ng/ml

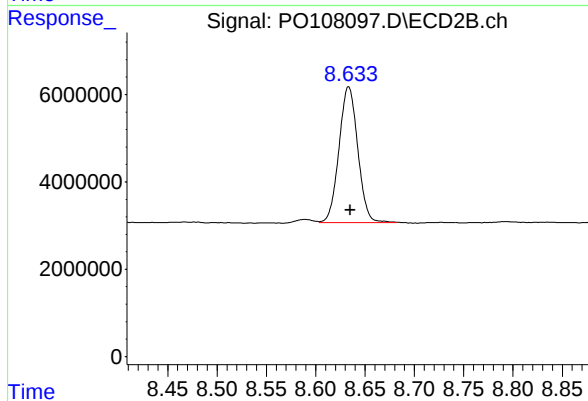

#2 Decachlorobiphenyl

R.T.: 8.633 min
Delta R.T.: -0.002 min
Response: 41123449
Conc: 12.09 ng/ml m