

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111925\
 Data File : PO115225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2025 16:57
 Operator : YP/AJ
 Sample : Q3667-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RIGHT-SIDE-WALL

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/20/2025
 Supervised By :Sohil Jodhani 11/20/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 01:45:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.342	3.645	157.5E6	99349607	22.384	22.242
2) SA Decachlor...	9.919	8.632	100.1E6	87382114	22.645m	22.384

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111925\
Data File : PO115225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2025 16:57
Operator : YP/AJ
Sample : Q3667-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RIGHT-SIDE-WALL


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/20/2025
Supervised By :Sohil Jodhani 11/20/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 01:45:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

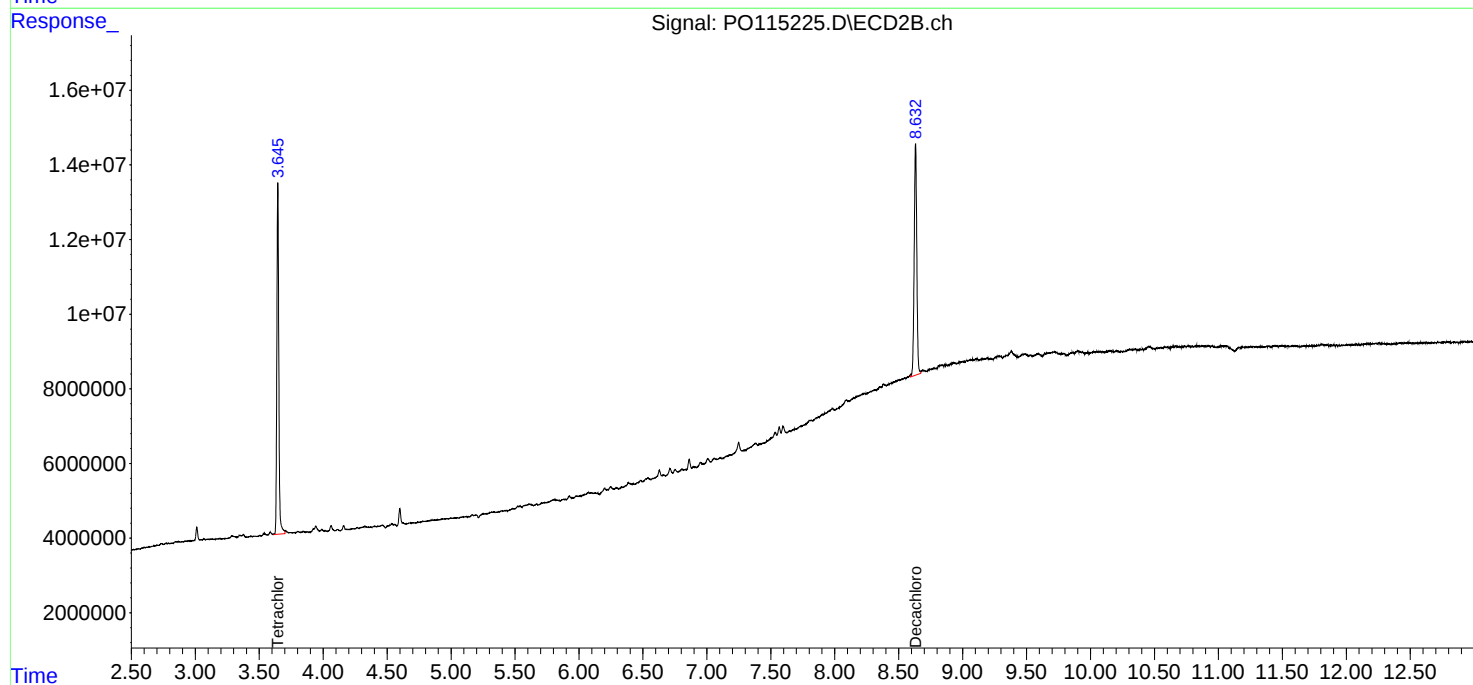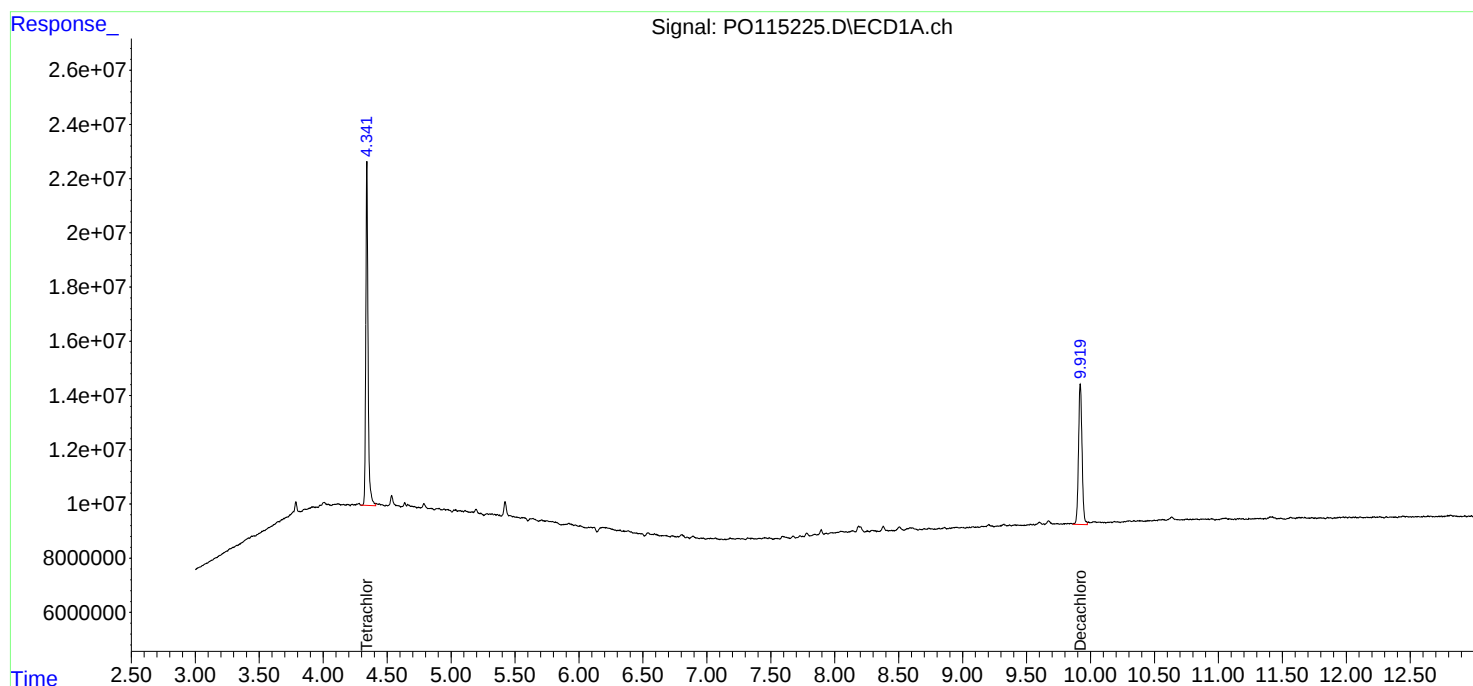

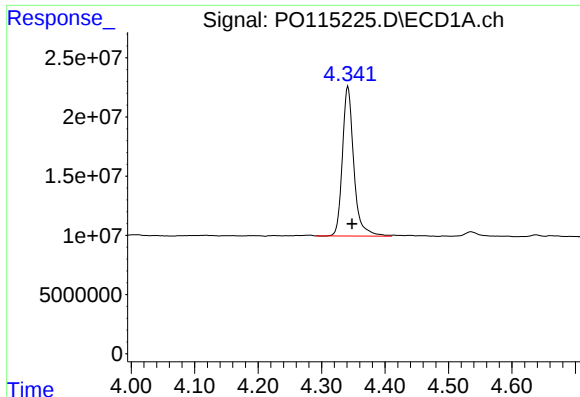


#1 Tetrachloro-m-xylene

R.T.: 4.342 min
Delta R.T.: -0.006 min
Response: 157544063
Conc: 22.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
RIGHT-SIDE-WALL


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/20/2025
Supervised By :Sohil Jodhani 11/20/2025

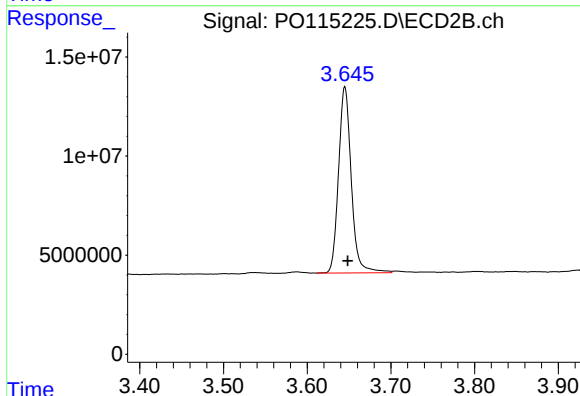


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.003 min
Response: 99349607
Conc: 22.24 ng/ml

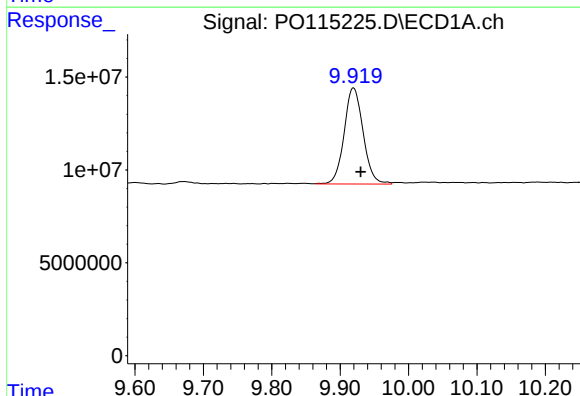

#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.011 min
Response: 100098187
Conc: 22.65 ng/ml m

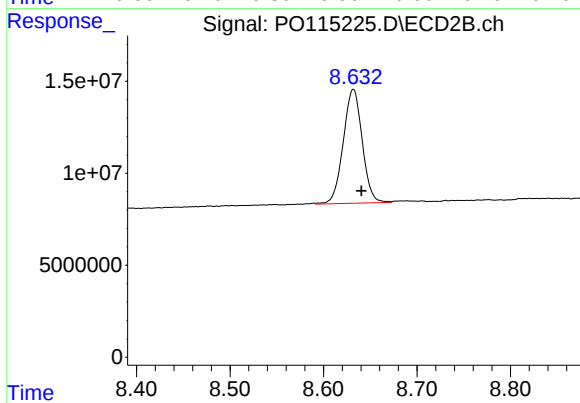

#2 Decachlorobiphenyl

R.T.: 8.632 min
Delta R.T.: -0.009 min
Response: 87382114
Conc: 22.38 ng/ml