

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112019\
 Data File : P0063906.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2019 10:15
 Operator : SM/AJ
 Sample : K5826-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-15-S

Manual Integrations
 APPROVED

Ankita
 11/21/2019 1:36:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 11:01:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.567	854419	657136	27.945	29.586
2)	SA Decachlor...	9.942	8.536	983289	793593	24.198	27.134
Target Compounds							
31)	L7 AR-1260-1	7.070	6.119	49315	40339	24.436m	25.687
32)	L7 AR-1260-2	7.326	6.305	67288	49952	26.708	25.393
33)	L7 AR-1260-3	7.684	6.459	53643	41281	26.475	23.146
34)	L7 AR-1260-4	7.908	6.929	66974	38506	28.123	24.457
35)	L7 AR-1260-5	8.219	7.169	102312	90898	21.795	23.446

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112019\
Data File : PO063906.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2019 10:15
Operator : SM/AJ
Sample : K5826-03
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-15-S


Manual Integrations
APPROVED

Ankita
11/21/2019 1:36:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 11:01:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

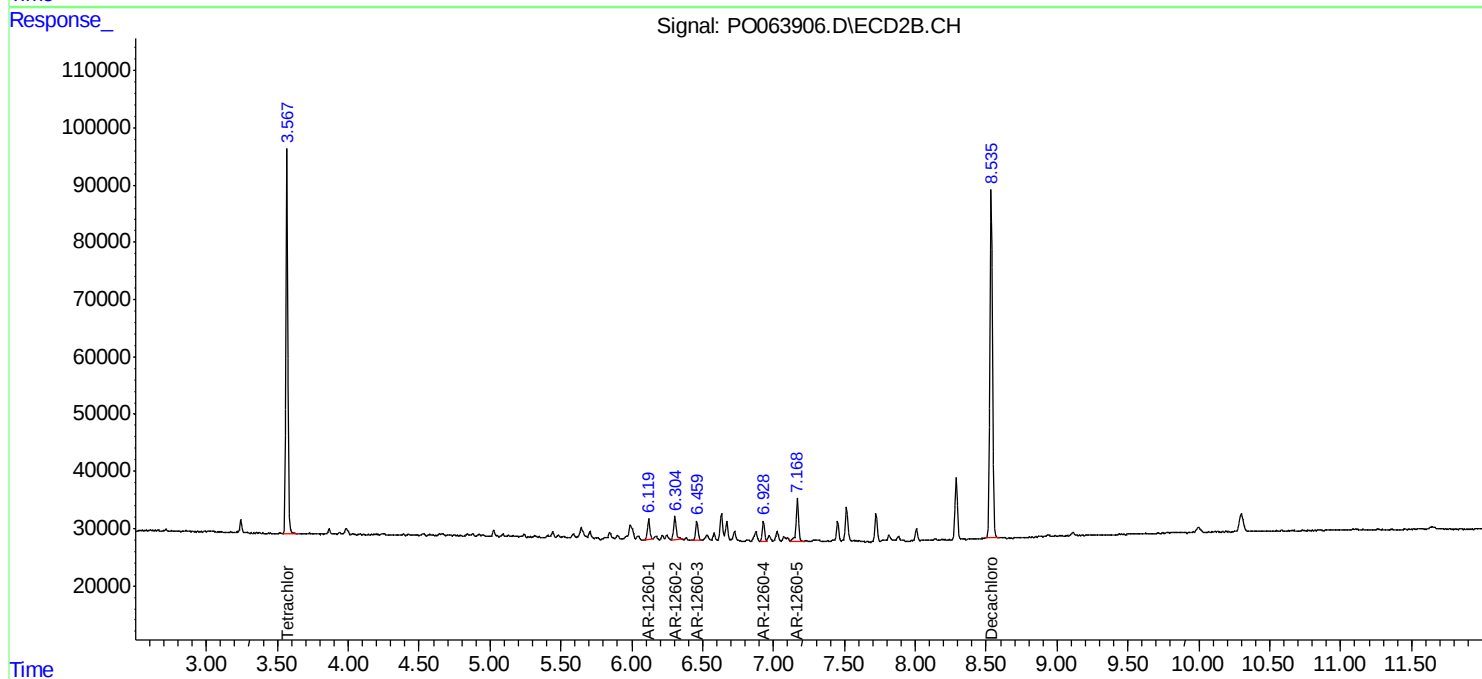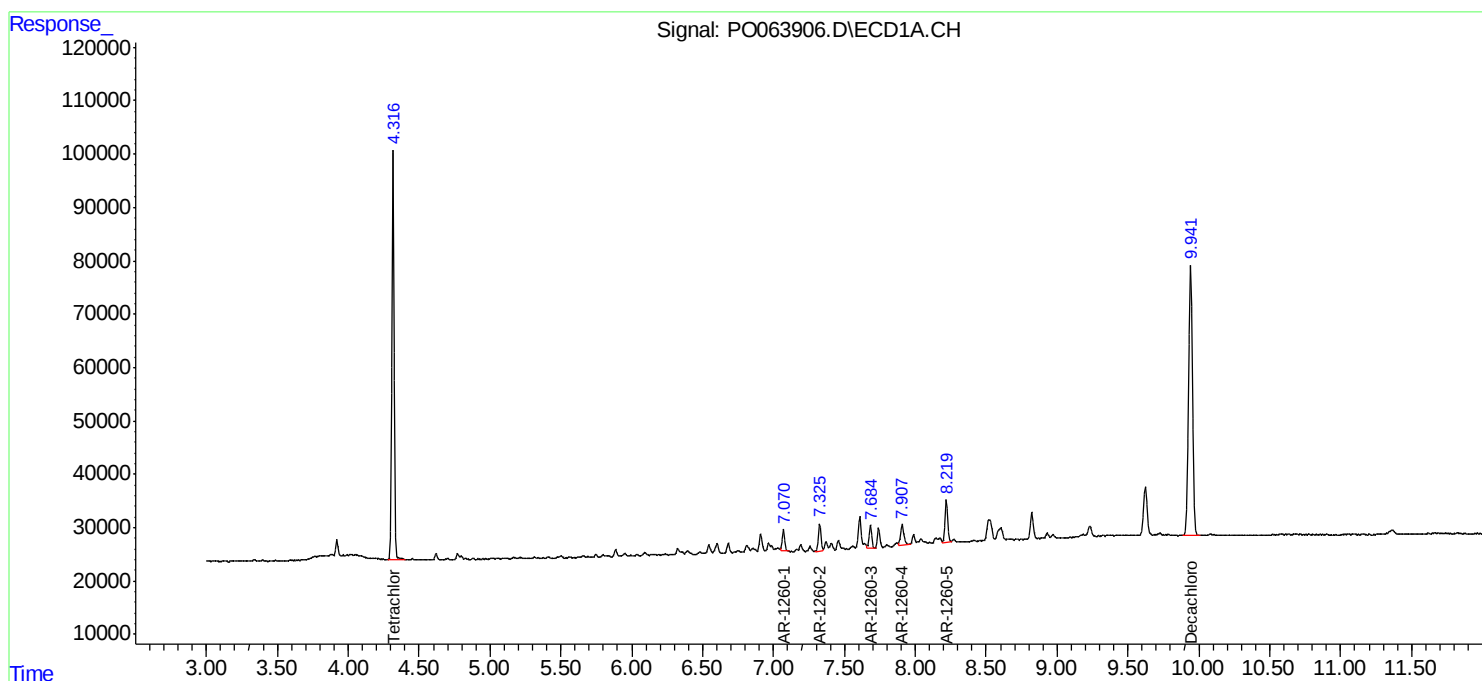

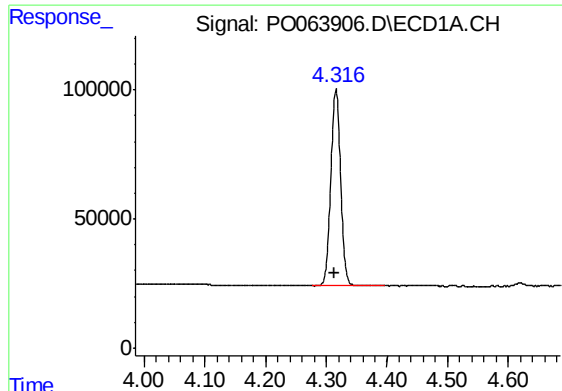


#1 Tetrachloro-m-xylene

R.T.: 4.316 min
Delta R.T.: 0.002 min
Response: 854419
Conc: 27.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-15-S


Manual Integrations
APPROVED

Ankita
11/21/2019 1:36:29 PM

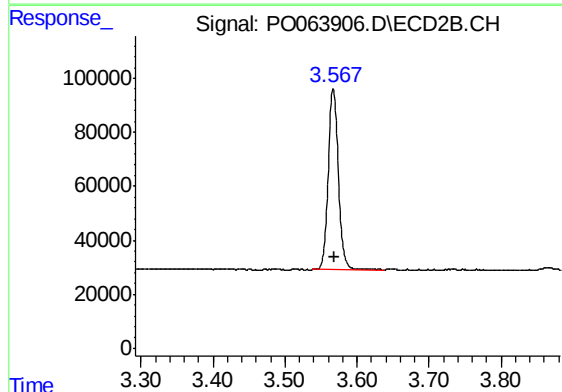


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: -0.002 min
Response: 657136
Conc: 29.59 ng/ml

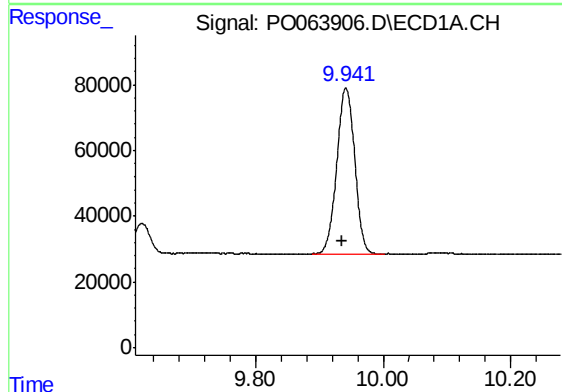


#2 Decachlorobiphenyl

R.T.: 9.942 min
Delta R.T.: 0.006 min
Response: 983289
Conc: 24.20 ng/ml

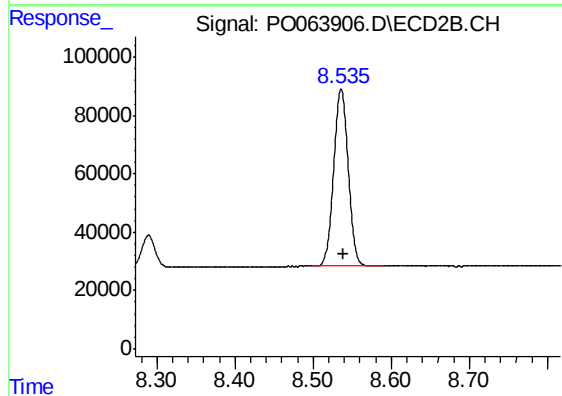

#2 Decachlorobiphenyl

R.T.: 8.536 min
Delta R.T.: -0.004 min
Response: 793593
Conc: 27.13 ng/ml

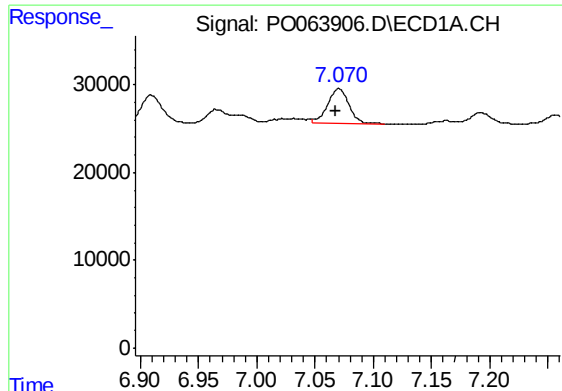


#31 AR-1260-1

R.T.: 7.070 min
Delta R.T.: 0.003 min
Response: 49315
Conc: 24.44 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-15-S


Manual Integrations
APPROVED

Ankita
11/21/2019 1:36:29 PM

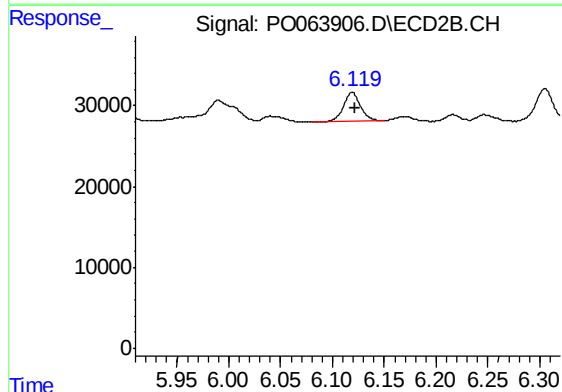


#31 AR-1260-1

R.T.: 6.119 min
Delta R.T.: -0.002 min
Response: 40339
Conc: 25.69 ng/ml

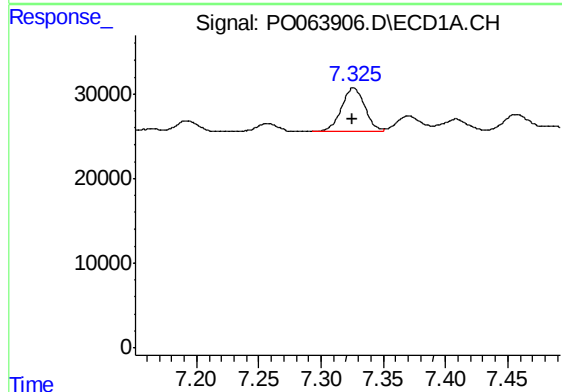


#32 AR-1260-2

R.T.: 7.326 min
Delta R.T.: 0.001 min
Response: 67288
Conc: 26.71 ng/ml

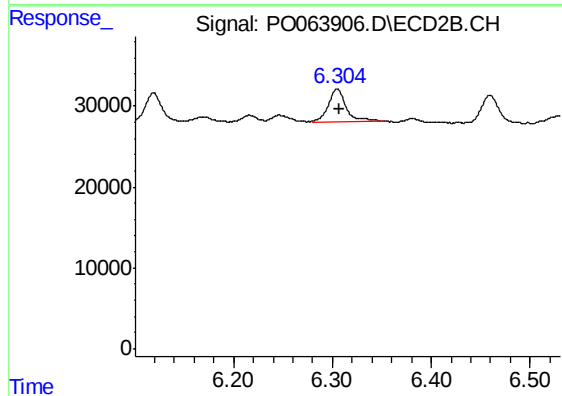

#32 AR-1260-2

R.T.: 6.305 min
Delta R.T.: -0.003 min
Response: 49952
Conc: 25.39 ng/ml

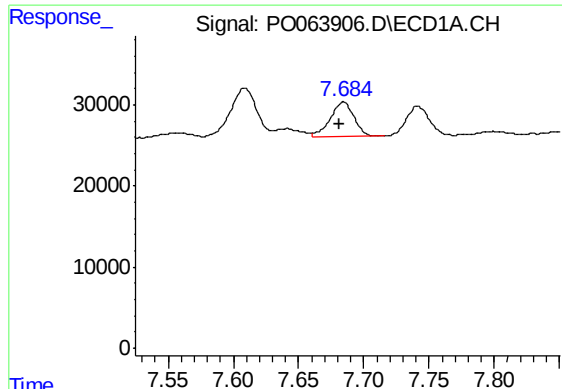


#33 AR-1260-3

R.T.: 7.684 min
Delta R.T.: 0.002 min
Response: 53643
Conc: 26.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-15-S


Manual Integrations
APPROVED

Ankita
11/21/2019 1:36:29 PM

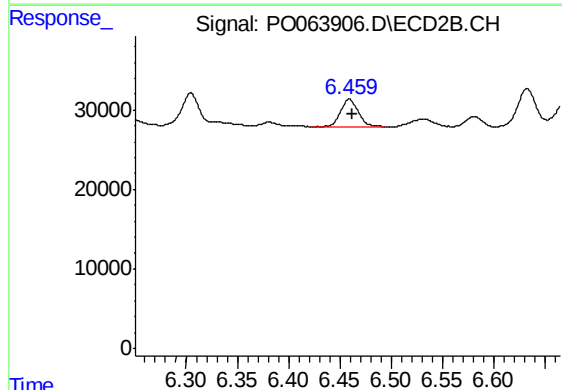


#33 AR-1260-3

R.T.: 6.459 min
Delta R.T.: -0.002 min
Response: 41281
Conc: 23.15 ng/ml

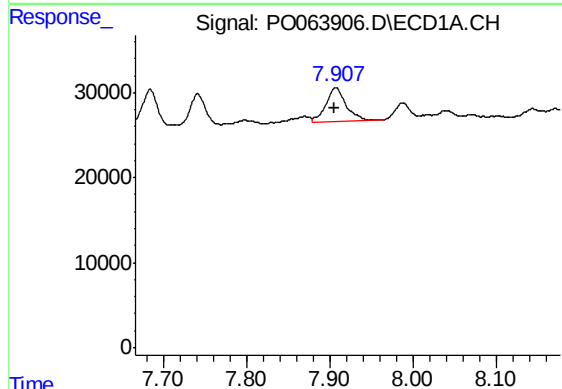


#34 AR-1260-4

R.T.: 7.908 min
Delta R.T.: 0.003 min
Response: 66974
Conc: 28.12 ng/ml

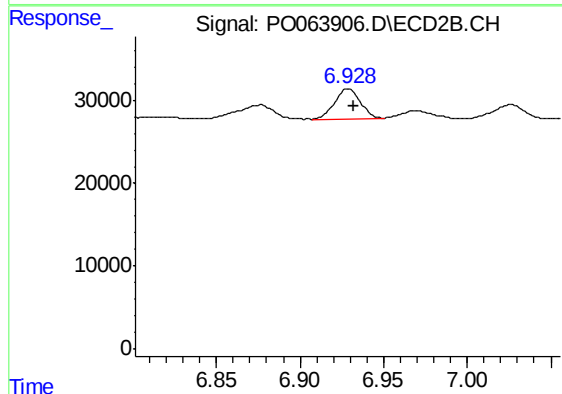

#34 AR-1260-4

R.T.: 6.929 min
Delta R.T.: -0.003 min
Response: 38506
Conc: 24.46 ng/ml

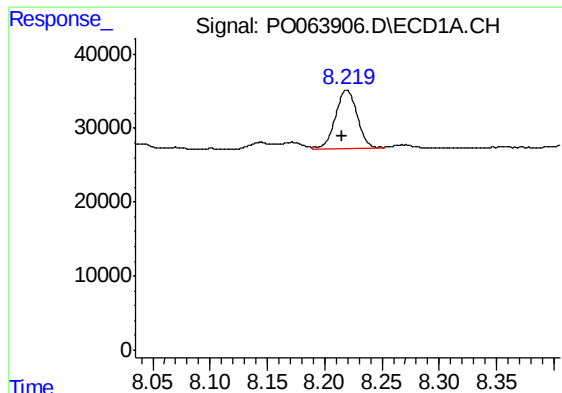


#35 AR-1260-5

R.T.: 8.219 min
Delta R.T.: 0.004 min
Response: 102312
Conc: 21.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-15-S

Manual Integrations
APPROVED

Ankita
11/21/2019 1:36:29 PM

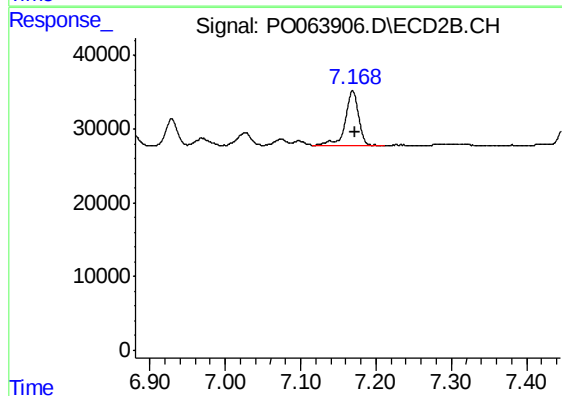

#35 AR-1260-5

R.T.: 7.169 min
Delta R.T.: -0.003 min
Response: 90898
Conc: 23.45 ng/ml