

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112019\
 Data File : P0063922.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2019 15:47
 Operator : SM/AJ
 Sample : K5927-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B-7

Manual Integrations
 APPROVED

Ankita
 11/21/2019 1:36:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 16:03:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.315	3.567	824189	659284	26.956	29.682
2)	SA Decachlor...	9.940	8.535	757466	565392	18.641	19.332
Target Compounds							
31)	L7 AR-1260-1	7.069	6.117	681331	612231	337.609	389.855
32)	L7 AR-1260-2	7.325	6.304	989543	707416	392.772	359.620
33)	L7 AR-1260-3	7.683	6.457	416795	587419	205.707	329.365 #
34)	L7 AR-1260-4	7.904	6.928	705524	304516	296.255	193.410 #
35)	L7 AR-1260-5	8.218	7.168	920879	825066	196.170	212.813m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112019\
Data File : PO063922.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2019 15:47
Operator : SM/AJ
Sample : K5927-09
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
B-7


Manual Integrations
APPROVED

Ankita
11/21/2019 1:36:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 16:03:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

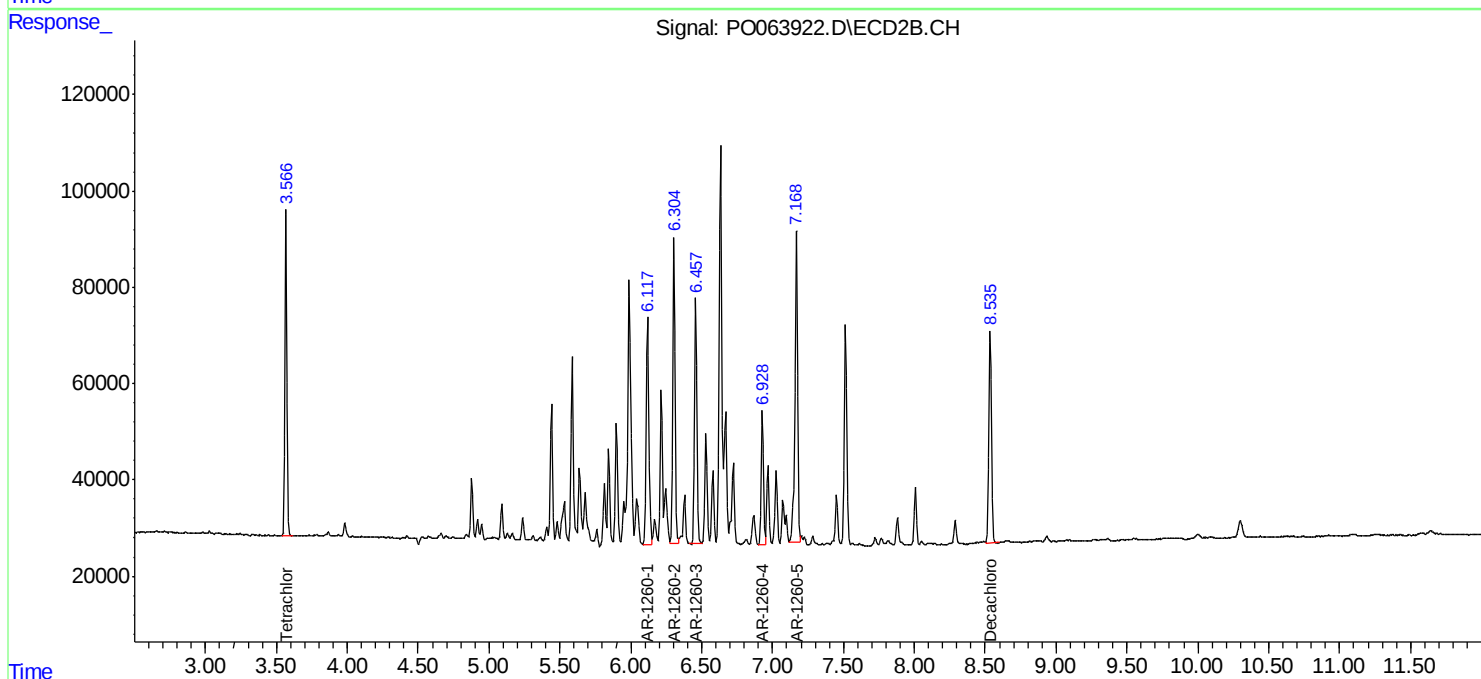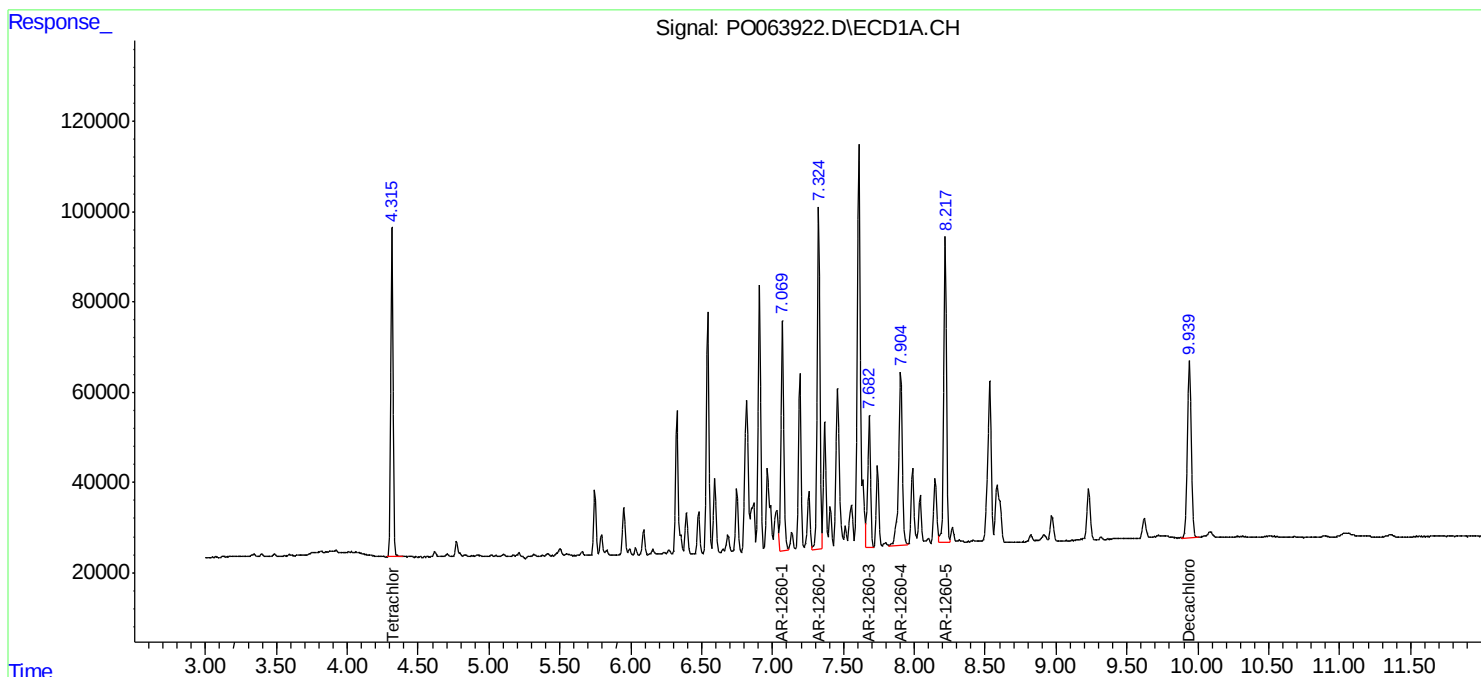

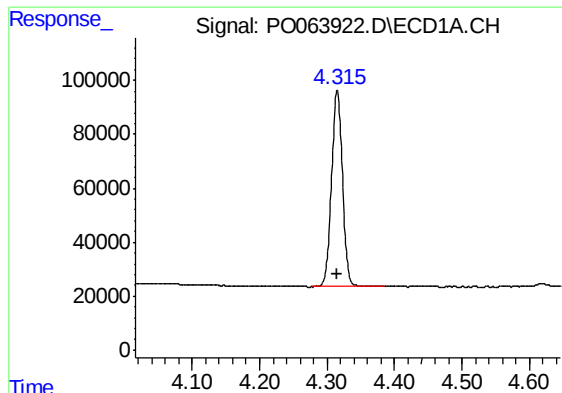


#1 Tetrachloro-m-xylene

R.T.: 4.315 min
Delta R.T.: 0.001 min
Response: 824189
Conc: 26.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
B-7


Manual Integrations
APPROVED

Ankita
11/21/2019 1:36:40 PM

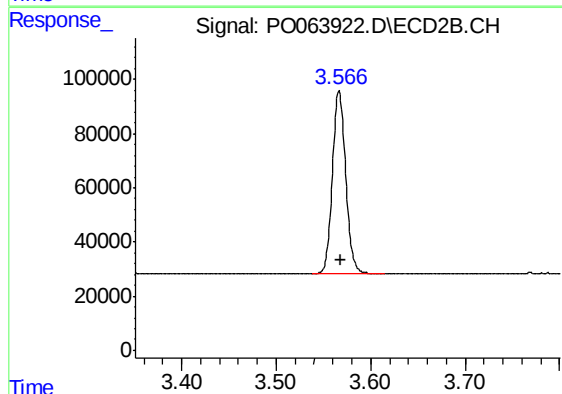


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: -0.002 min
Response: 659284
Conc: 29.68 ng/ml

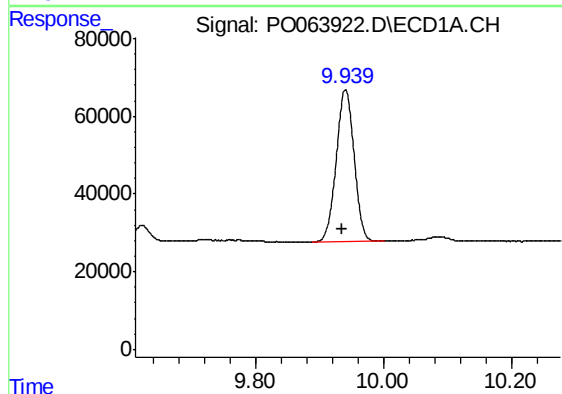


#2 Decachlorobiphenyl

R.T.: 9.940 min
Delta R.T.: 0.004 min
Response: 757466
Conc: 18.64 ng/ml

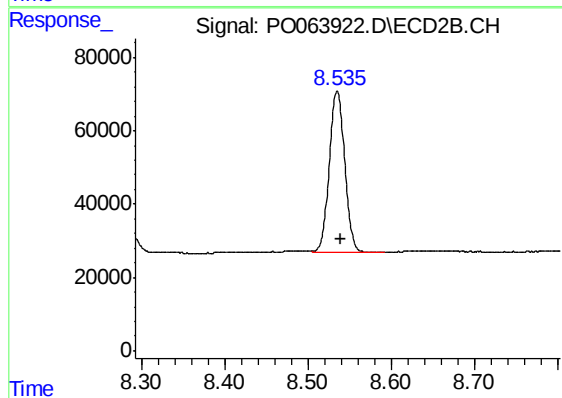

#2 Decachlorobiphenyl

R.T.: 8.535 min
Delta R.T.: -0.004 min
Response: 565392
Conc: 19.33 ng/ml

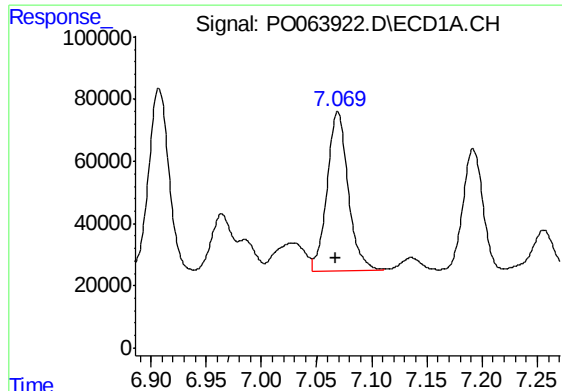


#31 AR-1260-1

R.T.: 7.069 min
Delta R.T.: 0.002 min
Response: 681331
Conc: 337.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
B-7


Manual Integrations
APPROVED

Ankita
11/21/2019 1:36:40 PM

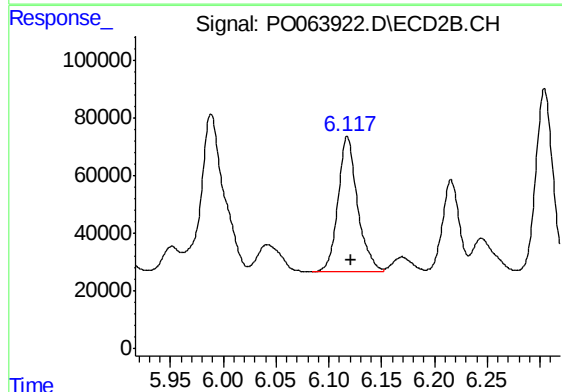


#31 AR-1260-1

R.T.: 6.117 min
Delta R.T.: -0.004 min
Response: 612231
Conc: 389.85 ng/ml

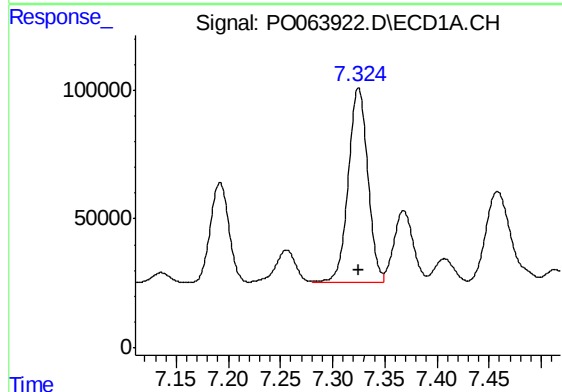


#32 AR-1260-2

R.T.: 7.325 min
Delta R.T.: 0.000 min
Response: 989543
Conc: 392.77 ng/ml

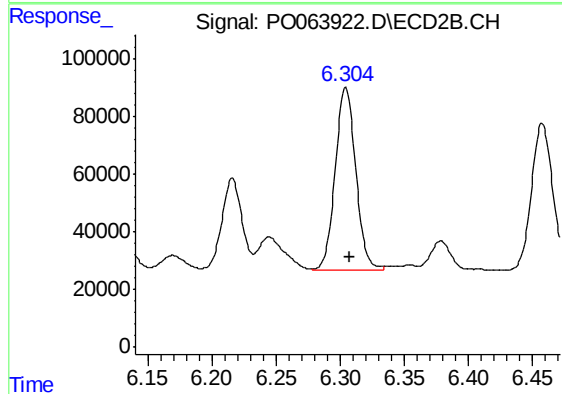

#32 AR-1260-2

R.T.: 6.304 min
Delta R.T.: -0.003 min
Response: 707416
Conc: 359.62 ng/ml

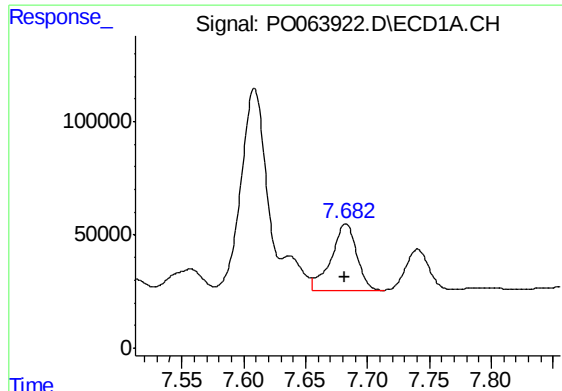


#33 AR-1260-3

R.T.: 7.683 min
Delta R.T.: 0.000 min
Response: 416795
Conc: 205.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
B-7


Manual Integrations
APPROVED

Ankita
11/21/2019 1:36:40 PM

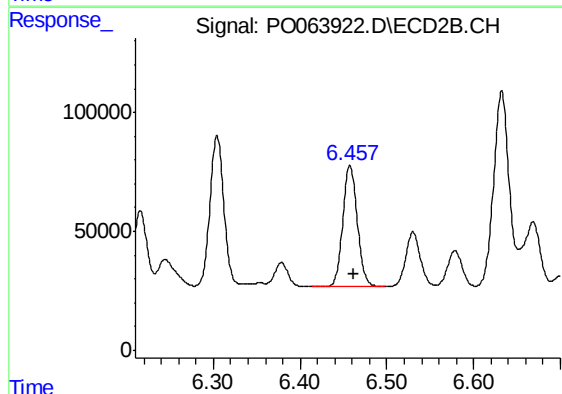


#33 AR-1260-3

R.T.: 6.457 min
Delta R.T.: -0.004 min
Response: 587419
Conc: 329.37 ng/ml

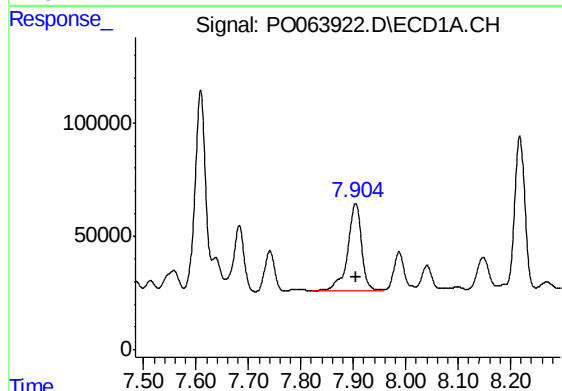


#34 AR-1260-4

R.T.: 7.904 min
Delta R.T.: 0.000 min
Response: 705524
Conc: 296.26 ng/ml

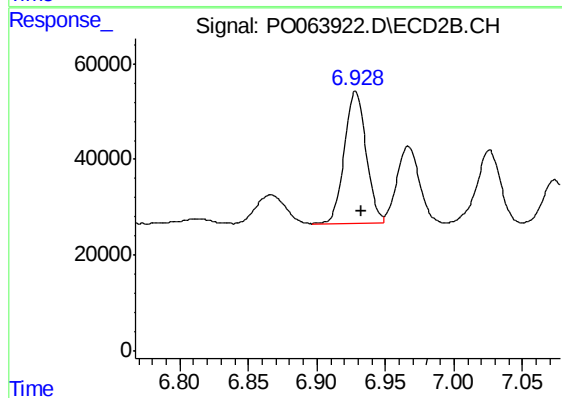

#34 AR-1260-4

R.T.: 6.928 min
Delta R.T.: -0.004 min
Response: 304516
Conc: 193.41 ng/ml

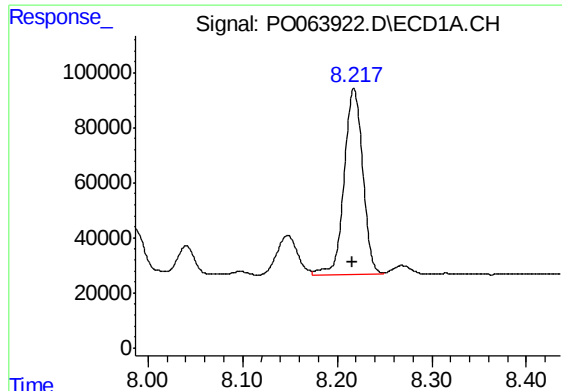


#35 AR-1260-5

R.T.: 8.218 min
Delta R.T.: 0.002 min
Response: 920879
Conc: 196.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
B-7

Manual Integrations
APPROVED

Ankita
11/21/2019 1:36:40 PM

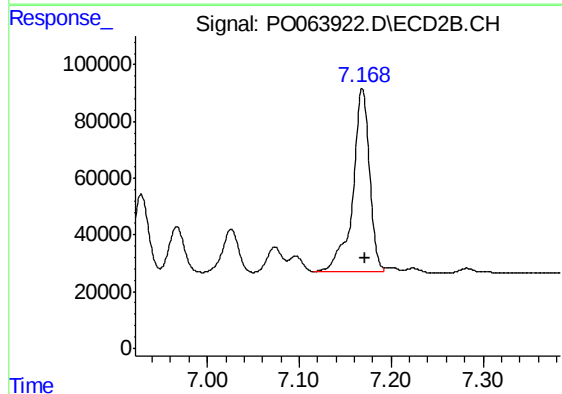

#35 AR-1260-5

R.T.: 7.168 min
Delta R.T.: -0.004 min
Response: 825066
Conc: 212.81 ng/ml m