

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112019\
Data File : P0063923.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2019 16:03
Operator : SM/AJ
Sample : K5927-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
B-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 16:21:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.315	3.566	791066	615927	25.873	27.730
2)	SA Decachlor...	9.940	8.535	784525	616783	19.307	21.089

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112019\
Data File : PO063923.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2019 16:03
Operator : SM/AJ
Sample : K5927-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
B-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 16:21:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

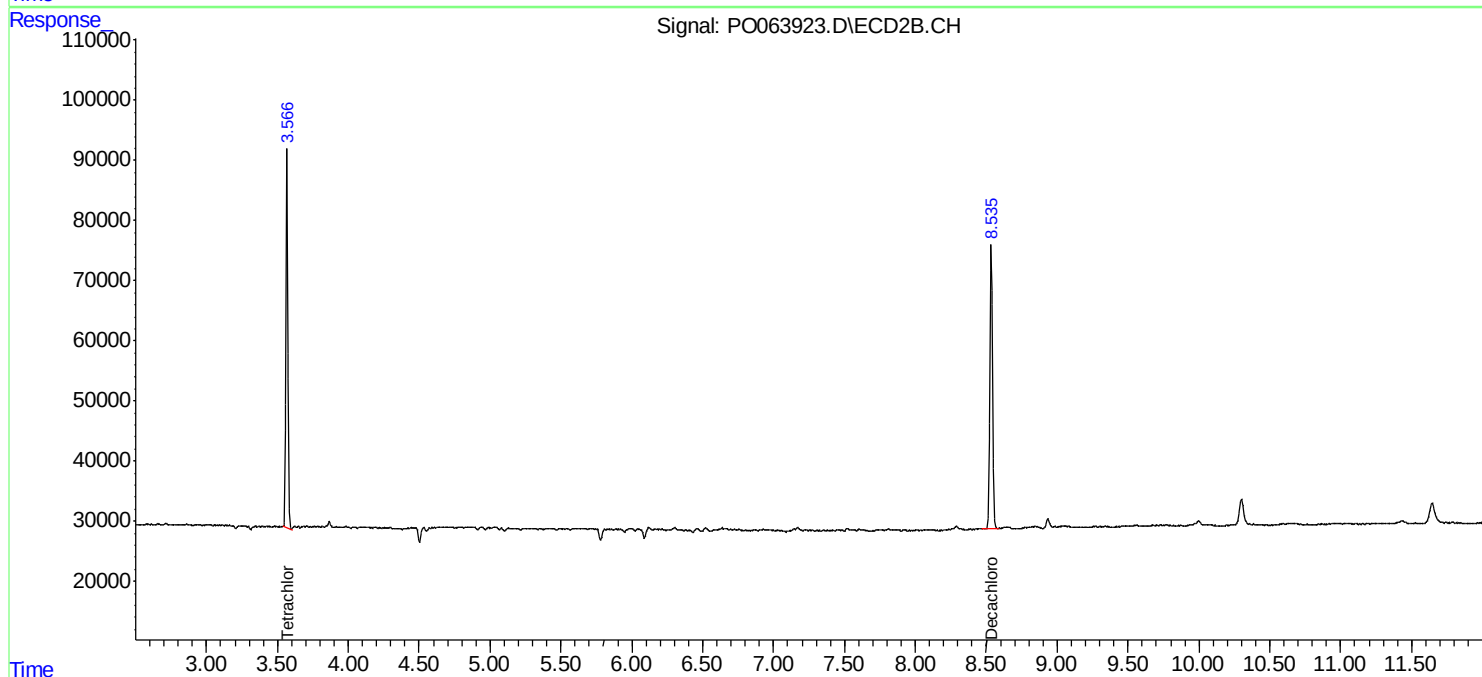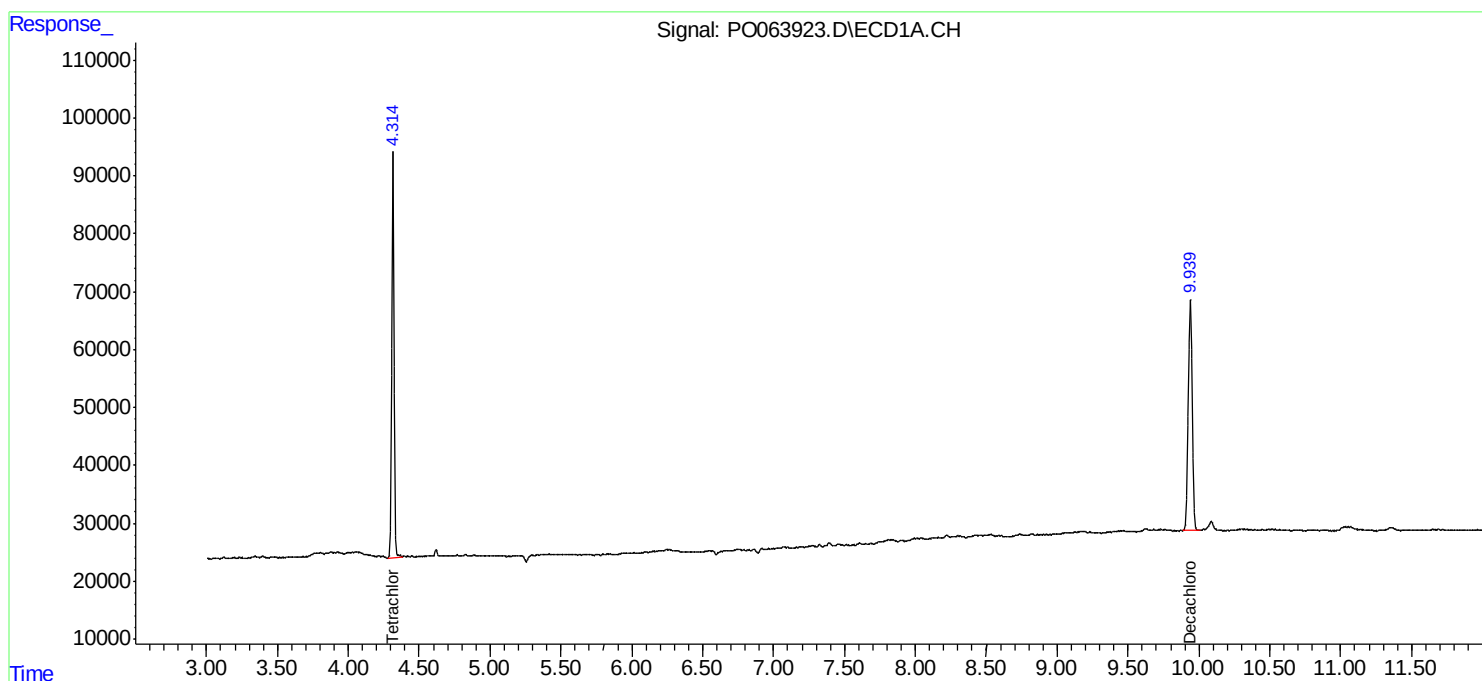


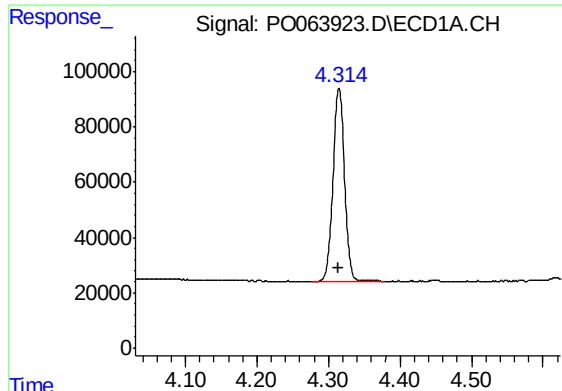

#1 Tetrachloro-m-xylene


R.T.: 4.315 min
Delta R.T.: 0.000 min
Response: 791066
Conc: 25.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
B-8

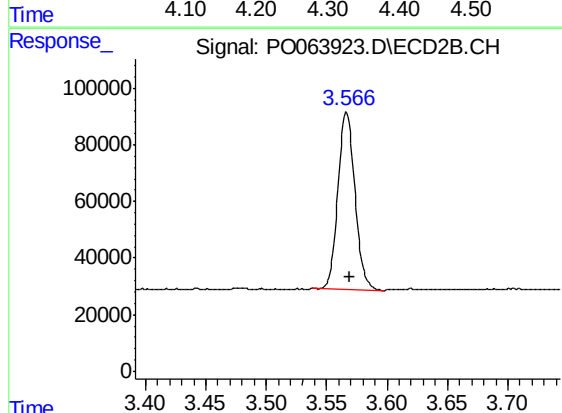


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.002 min
Response: 615927
Conc: 27.73 ng/ml

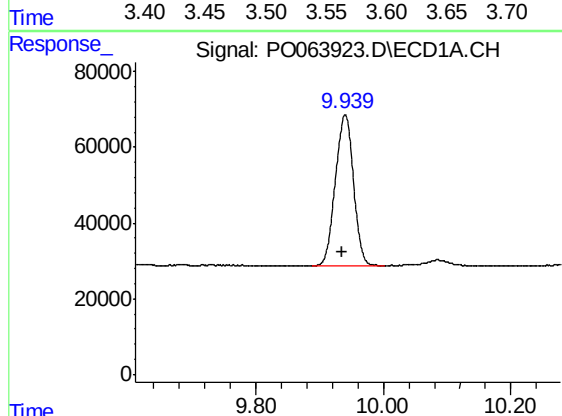

#2 Decachlorobiphenyl

R.T.: 9.940 min
Delta R.T.: 0.004 min
Response: 784525
Conc: 19.31 ng/ml

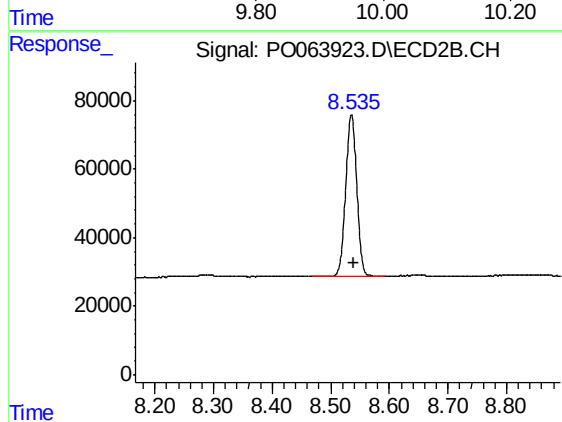

#2 Decachlorobiphenyl

R.T.: 8.535 min
Delta R.T.: -0.004 min
Response: 616783
Conc: 21.09 ng/ml