

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112020\
Data File : PO073403.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2020 20:51
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:59:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 19 12:09:14 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.946	4.012	1306980	768356	20.771	21.404
2) SA Decachlor...	10.979	9.281	1079564	635266	20.170	18.183

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112020\
Data File : PO073403.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2020 20:51
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:59:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 19 12:09:14 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

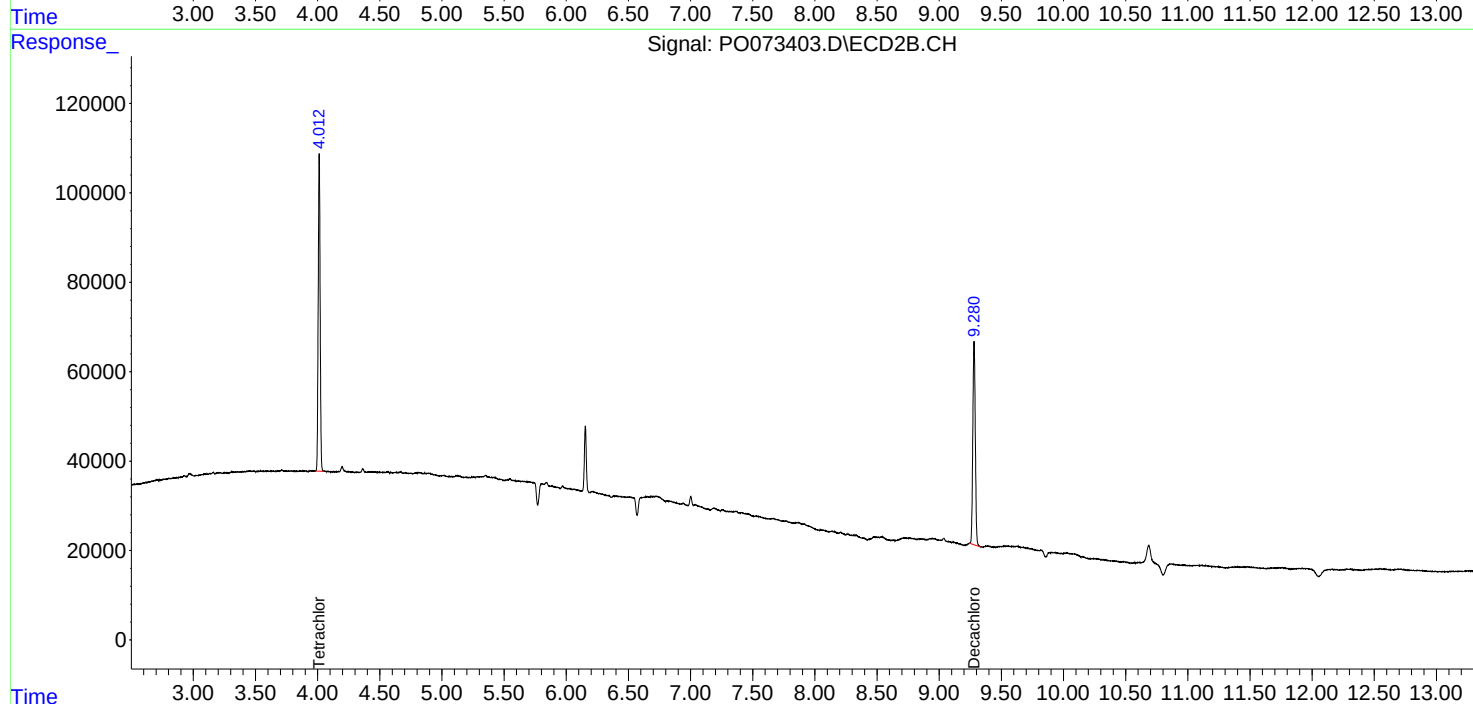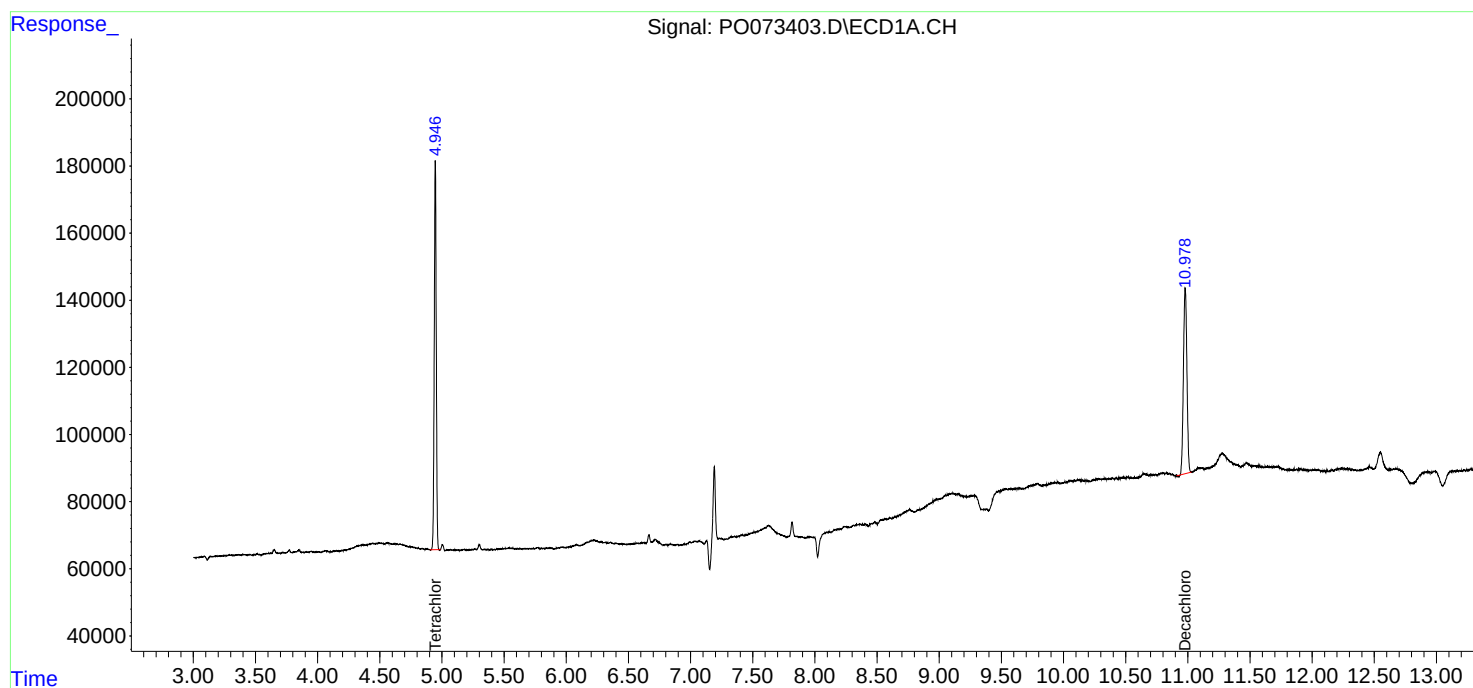


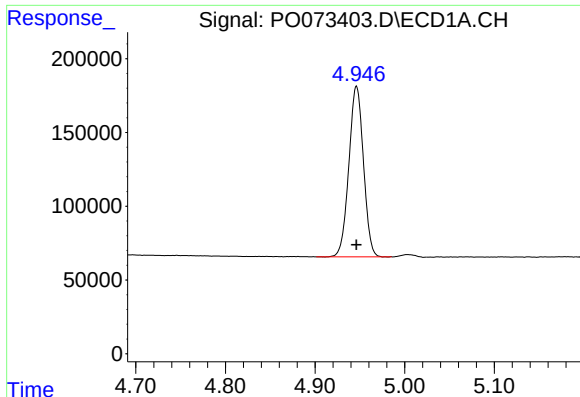

#1 Tetrachloro-m-xylene


R.T.: 4.946 min
Delta R.T.: 0.000 min
Response: 1306980
Conc: 20.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

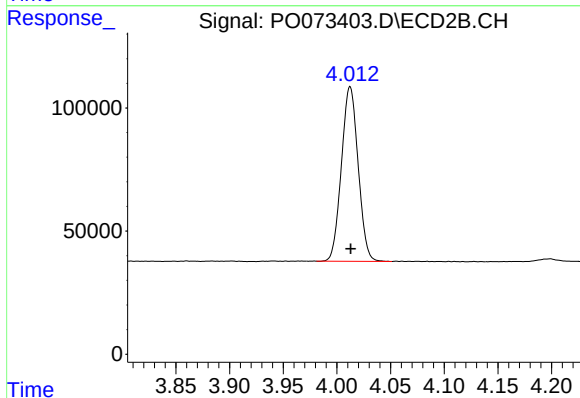


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 768356
Conc: 21.40 ng/ml

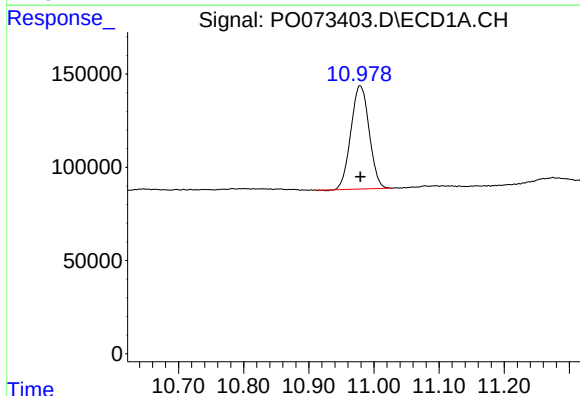

#2 Decachlorobiphenyl

R.T.: 10.979 min
Delta R.T.: 0.000 min
Response: 1079564
Conc: 20.17 ng/ml

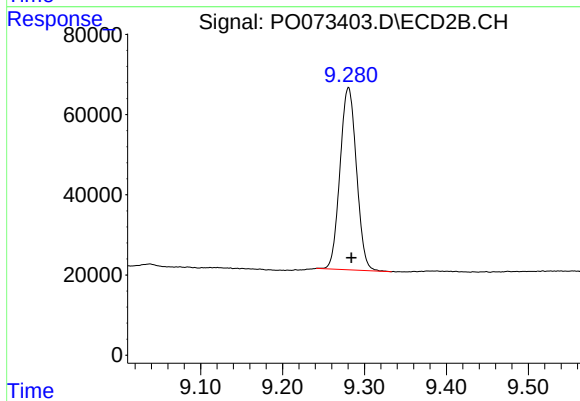

#2 Decachlorobiphenyl

R.T.: 9.281 min
Delta R.T.: -0.003 min
Response: 635266
Conc: 18.18 ng/ml