

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112024\
 Data File : P0108143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 17:16
 Operator : YP/AJ
 Sample : P4923-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 72-11991

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/21/2024
 Supervised By :Ankita Jodhani 11/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 01:10:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.637	120.5E6	62771421	13.837	18.514 #
2) SA Decachlor...	10.090	8.632	52922096	49134624	17.328	14.444m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112024\
Data File : PO108143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 17:16
Operator : YP/AJ
Sample : P4923-06
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
72-11991


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2024
Supervised By :Ankita Jodhani 11/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 01:10:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

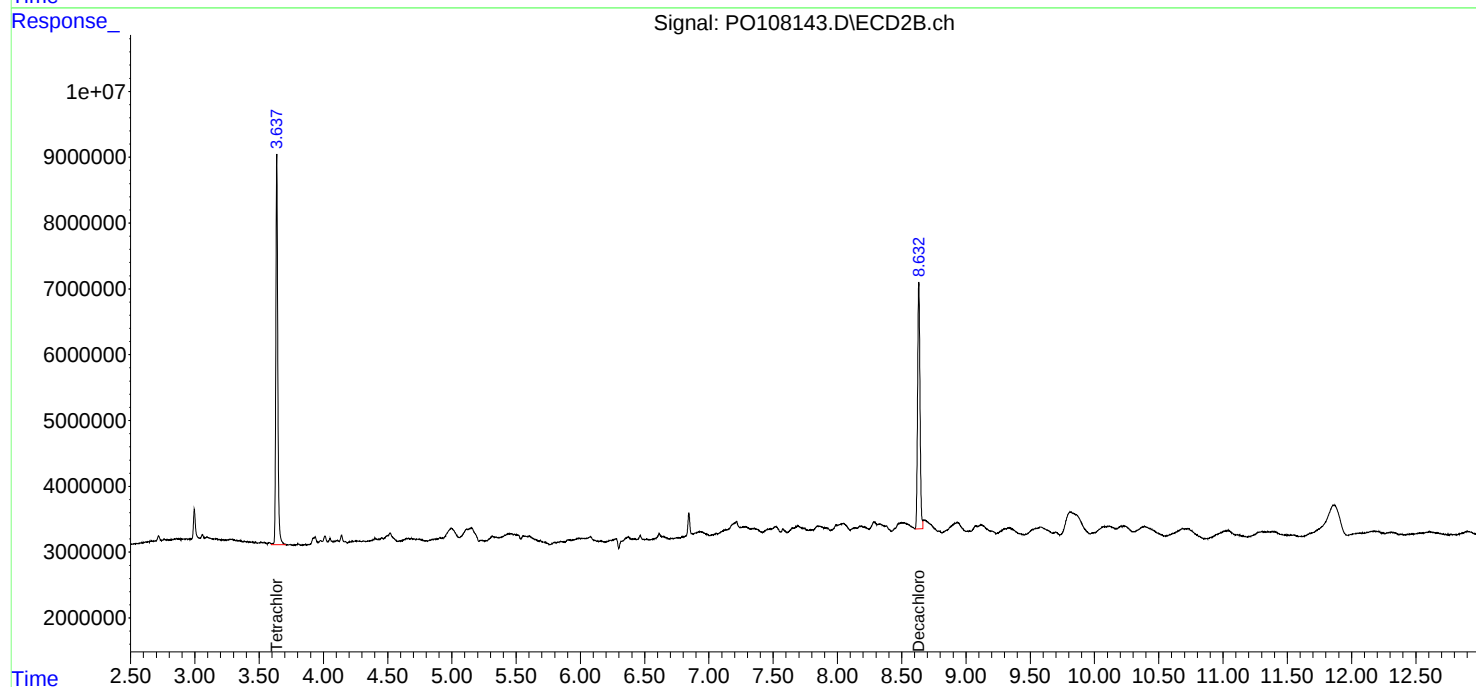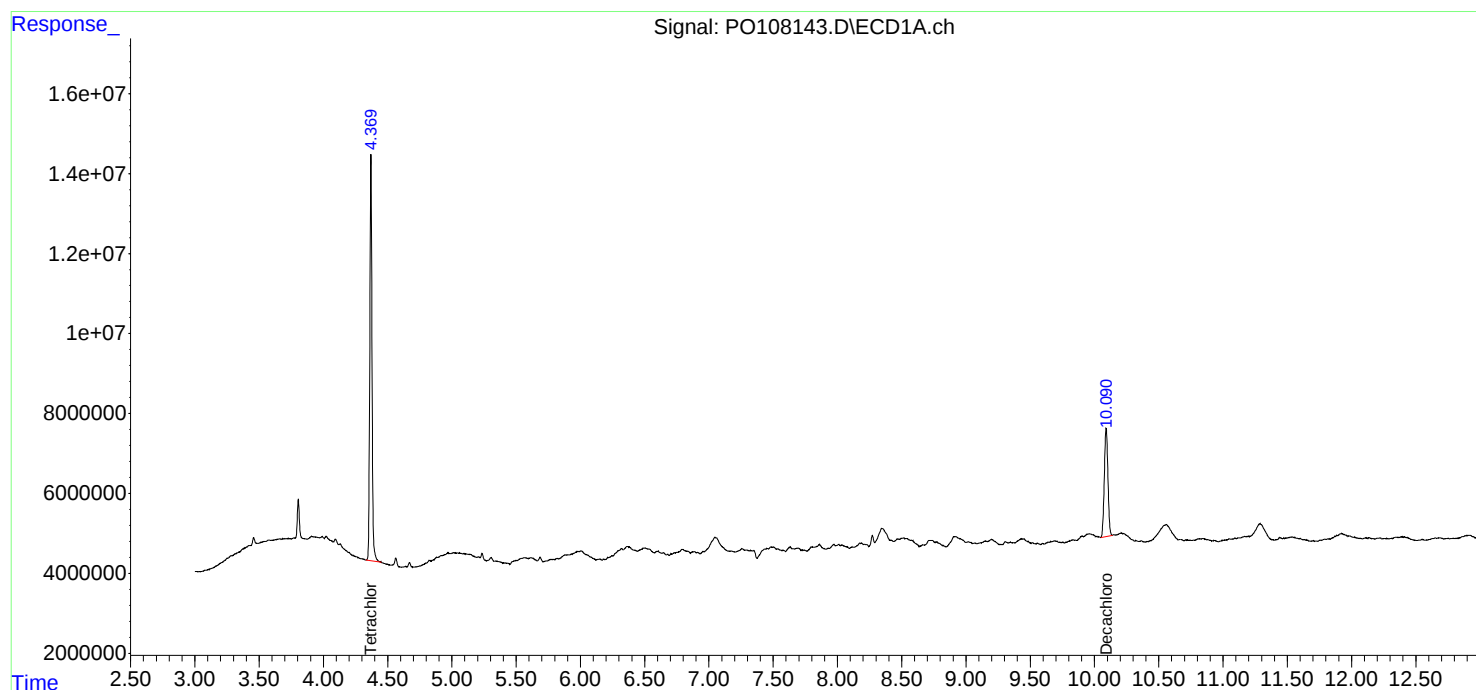

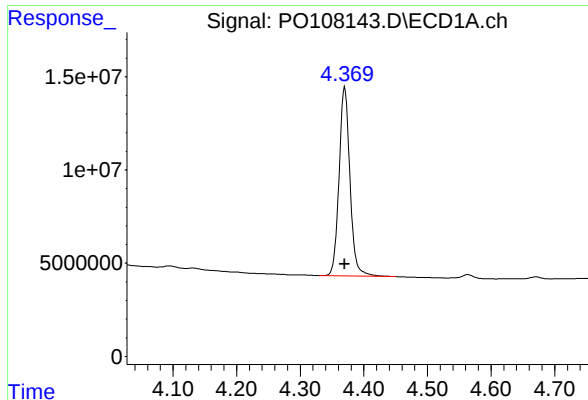


#1 Tetrachloro-m-xylene

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 120463663
Conc: 13.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
72-11991


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2024
Supervised By :Ankita Jodhani 11/21/2024

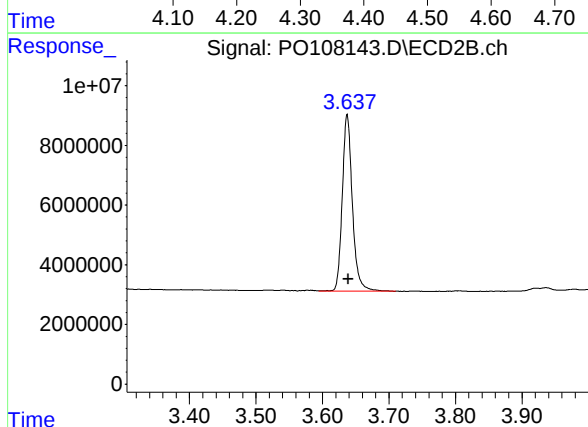


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 62771421
Conc: 18.51 ng/ml

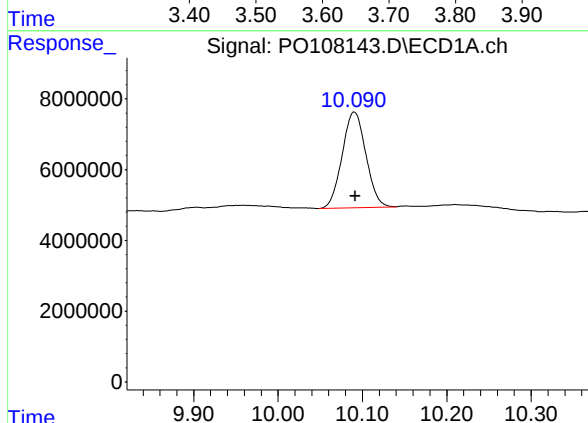

#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: 0.000 min
Response: 52922096
Conc: 17.33 ng/ml

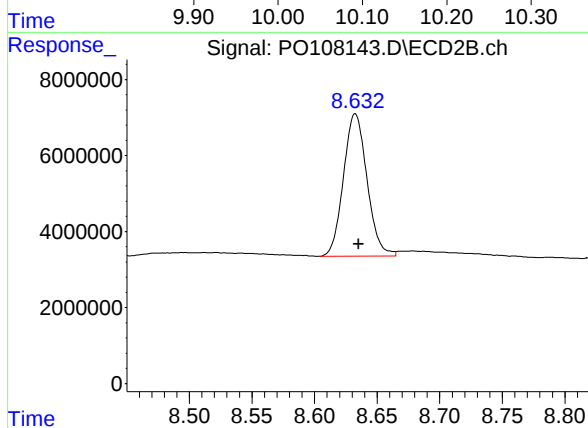

#2 Decachlorobiphenyl

R.T.: 8.632 min
Delta R.T.: -0.003 min
Response: 49134624
Conc: 14.44 ng/ml m