

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112024\
 Data File : P0108144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 17:33
 Operator : YP/AJ
 Sample : P4923-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SOM-24-00118

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/21/2024
 Supervised By :Ankita Jodhani 11/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 01:11:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.376	3.646	103.1E6	42193073	11.837	12.445
2) SA Decachlor...	10.093	8.633	63862587	60477500	20.910	17.779m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112024\
Data File : PO108144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 17:33
Operator : YP/AJ
Sample : P4923-09
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SOM-24-00118


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2024
Supervised By :Ankita Jodhani 11/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 01:11:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

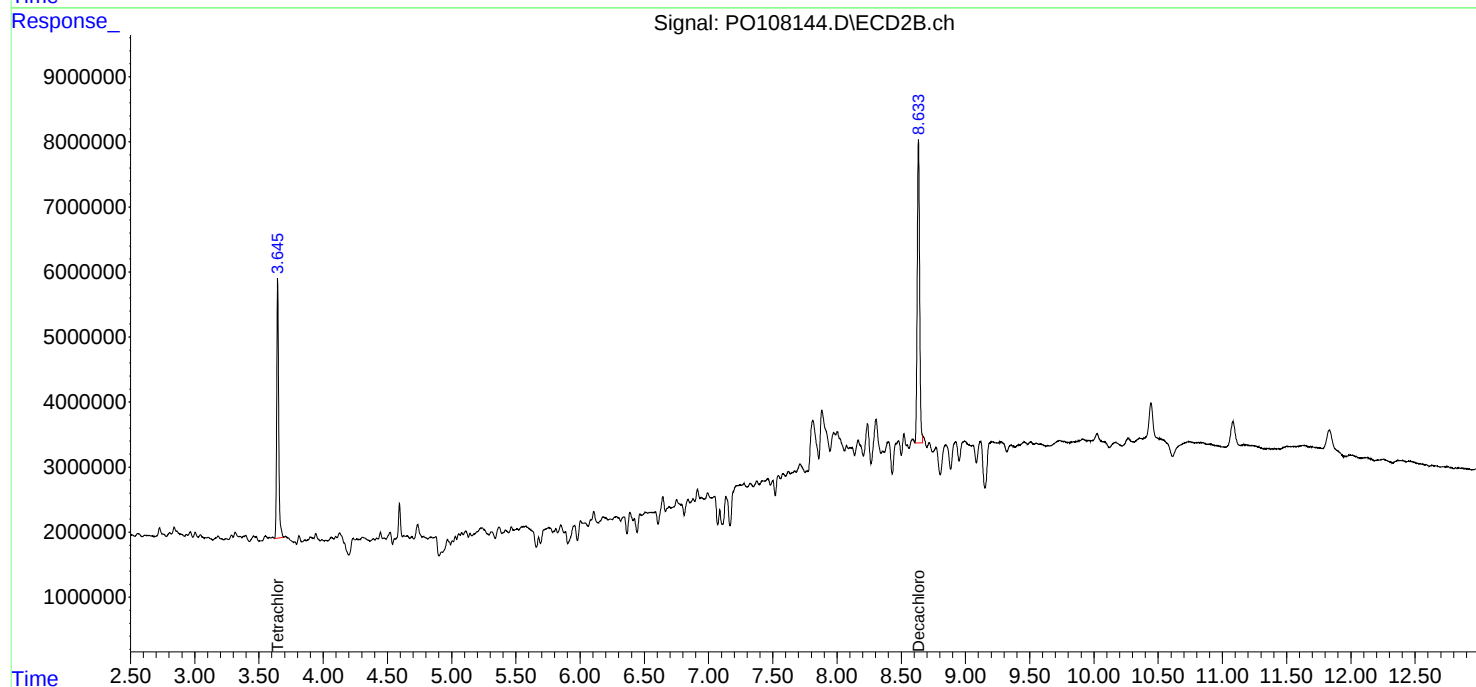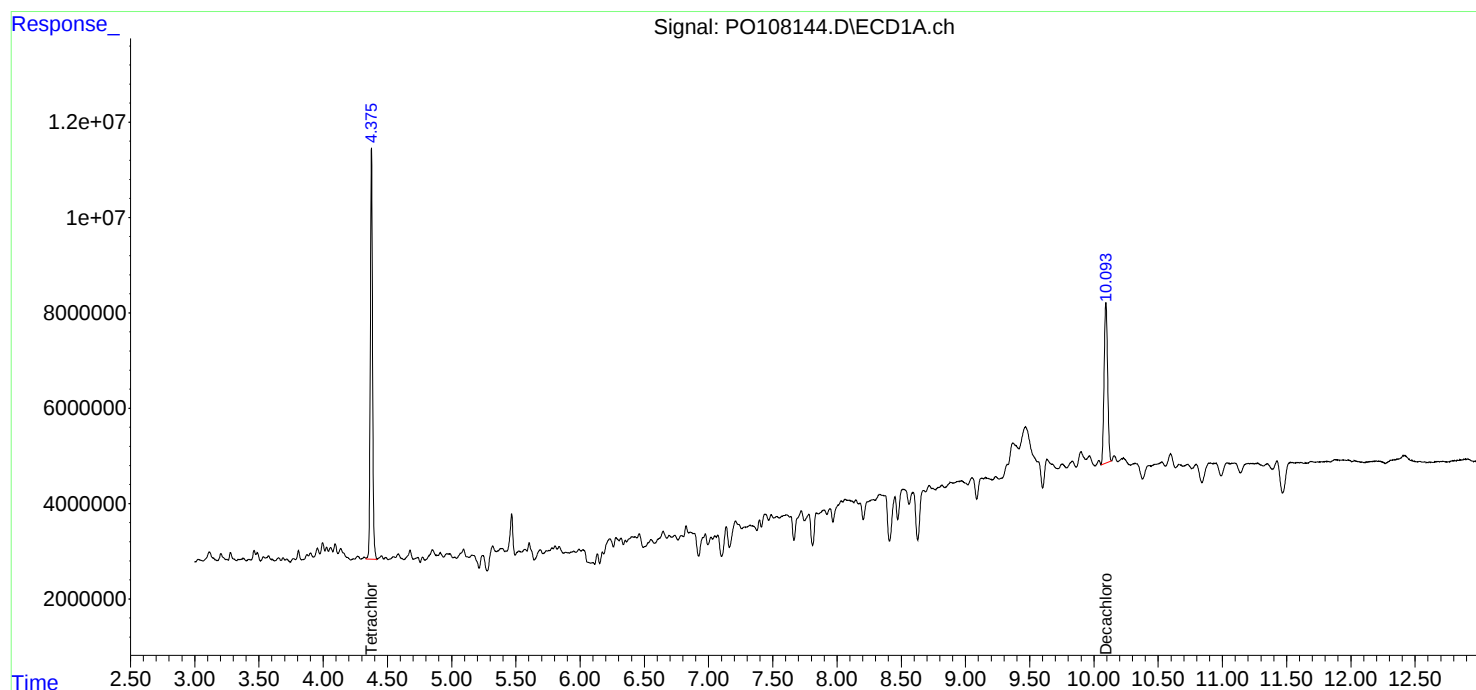

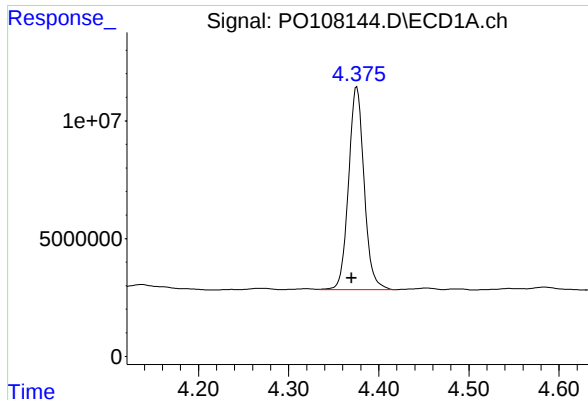


#1 Tetrachloro-m-xylene

R.T.: 4.376 min
Delta R.T.: 0.006 min
Response: 103055451
Conc: 11.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
SOM-24-00118


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2024
Supervised By :Ankita Jodhani 11/21/2024

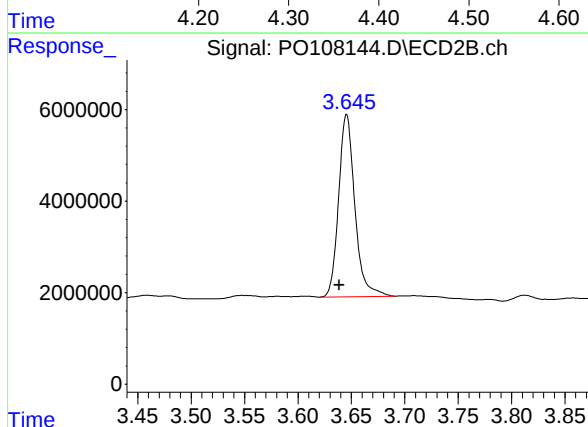


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.007 min
Response: 42193073
Conc: 12.44 ng/ml

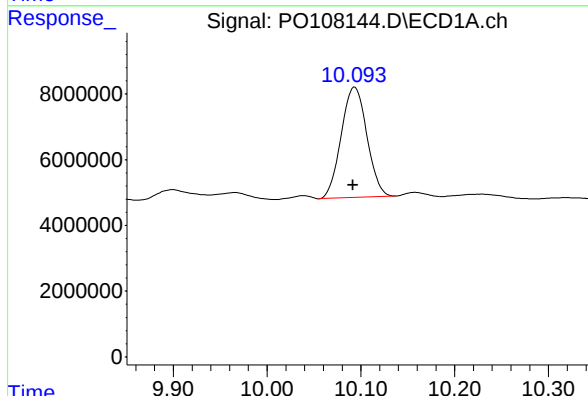

#2 Decachlorobiphenyl

R.T.: 10.093 min
Delta R.T.: 0.002 min
Response: 63862587
Conc: 20.91 ng/ml

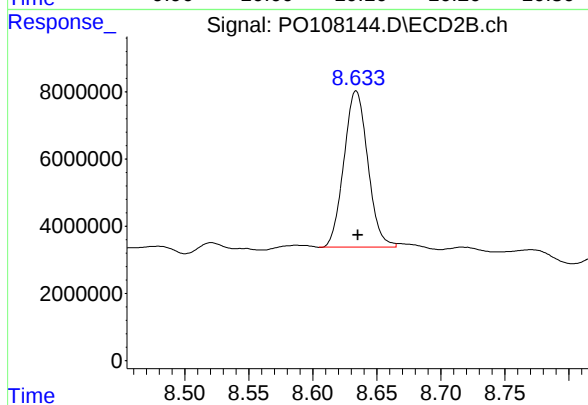

#2 Decachlorobiphenyl

R.T.: 8.633 min
Delta R.T.: -0.002 min
Response: 60477500
Conc: 17.78 ng/ml m