

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112025\
Data File : PO115264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2025 14:00
Operator : YP/AJ
Sample : Q3663-02 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2054

Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/21/2025
Supervised By :Sohil Jodhani 12/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 01:50:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.337	3.644	5665547	4788574	0.805m	1.072m#
2) SA Decachlor...	9.919	8.629	9209764	8927672	2.084	2.287

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112025\
Data File : PO115264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2025 14:00
Operator : YP/AJ
Sample : Q3663-02 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2054


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/21/2025
Supervised By :Sohil Jodhani 12/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 01:50:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

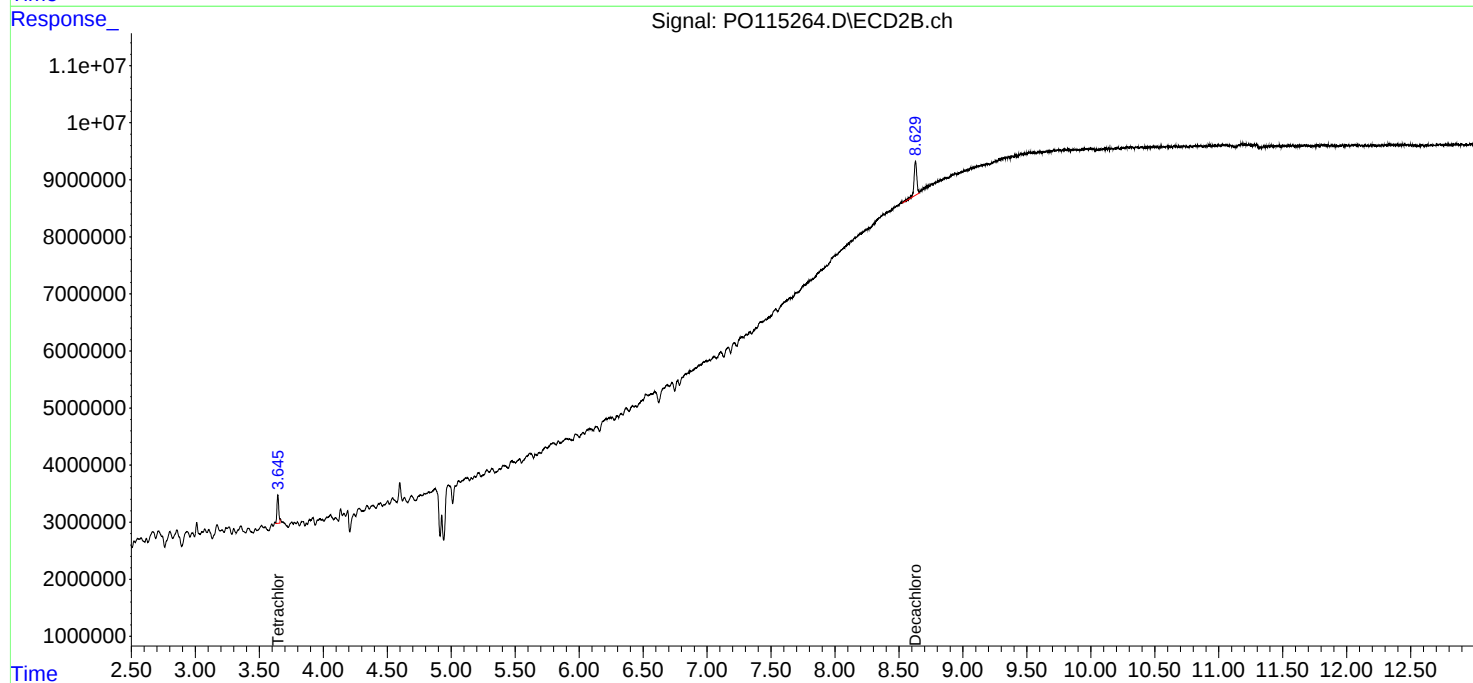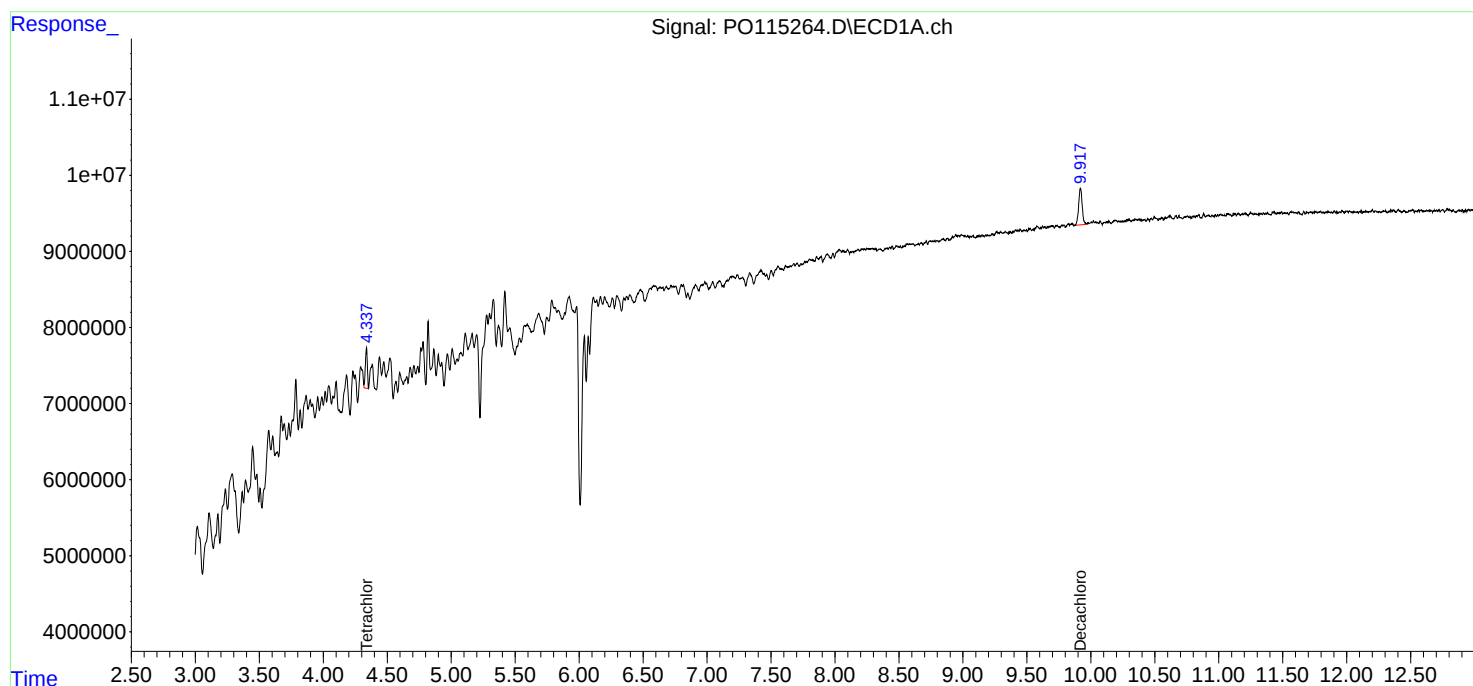

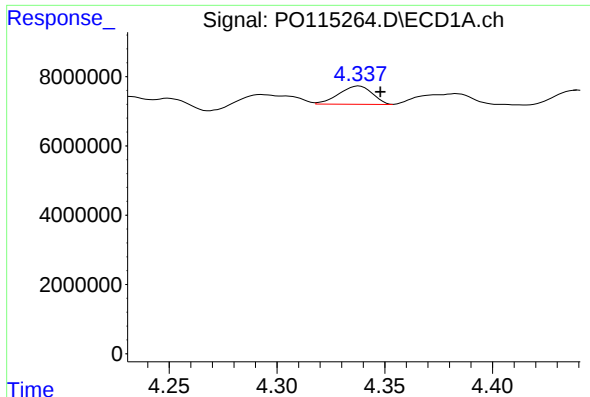


#1 Tetrachloro-m-xylene

R.T.: 4.337 min
Delta R.T.: -0.011 min
Response: 5665547
Conc: 0.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
2054


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/21/2025
Supervised By :Sohil Jodhani 12/01/2025

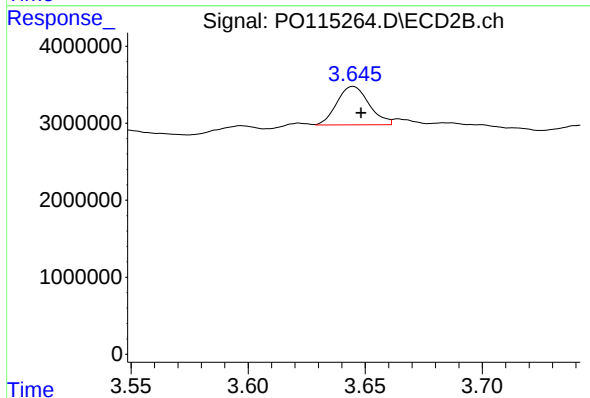


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.004 min
Response: 4788574
Conc: 1.07 ng/ml m

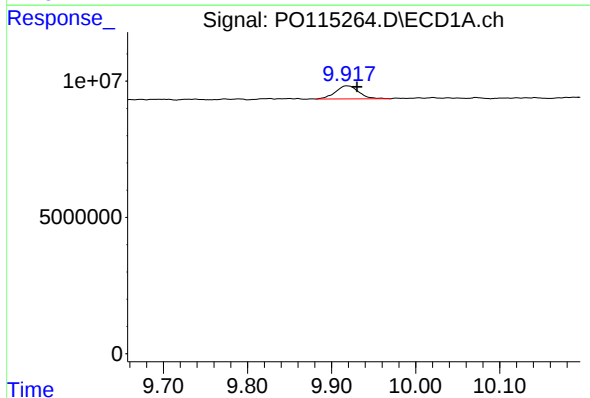

#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.011 min
Response: 9209764
Conc: 2.08 ng/ml

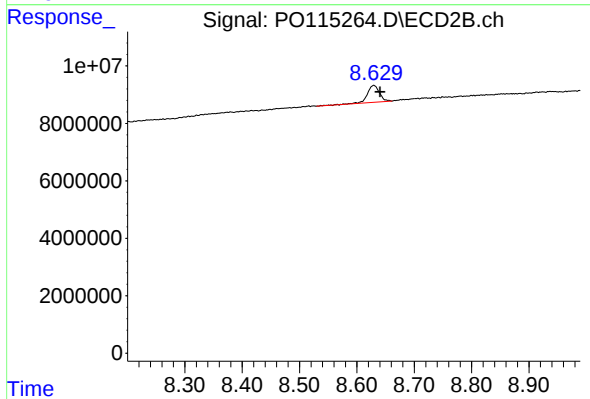

#2 Decachlorobiphenyl

R.T.: 8.629 min
Delta R.T.: -0.011 min
Response: 8927672
Conc: 2.29 ng/ml