

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112025\
 Data File : PO115297.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2025 03:09
 Operator : YP/AJ
 Sample : Q3666-02 10X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BUR-25-0102

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/01/2025
 Supervised By :Sohil Jodhani 12/01/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 03:41:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.337	3.643	17892977	21198532	2.542m	4.746m#
2) SA Decachlor...	9.916	8.629	13348669	12265262	3.020	3.142

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112025\
Data File : PO115297.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2025 03:09
Operator : YP/AJ
Sample : Q3666-02 10X
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BUR-25-0102


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/01/2025
Supervised By :Sohil Jodhani 12/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 03:41:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

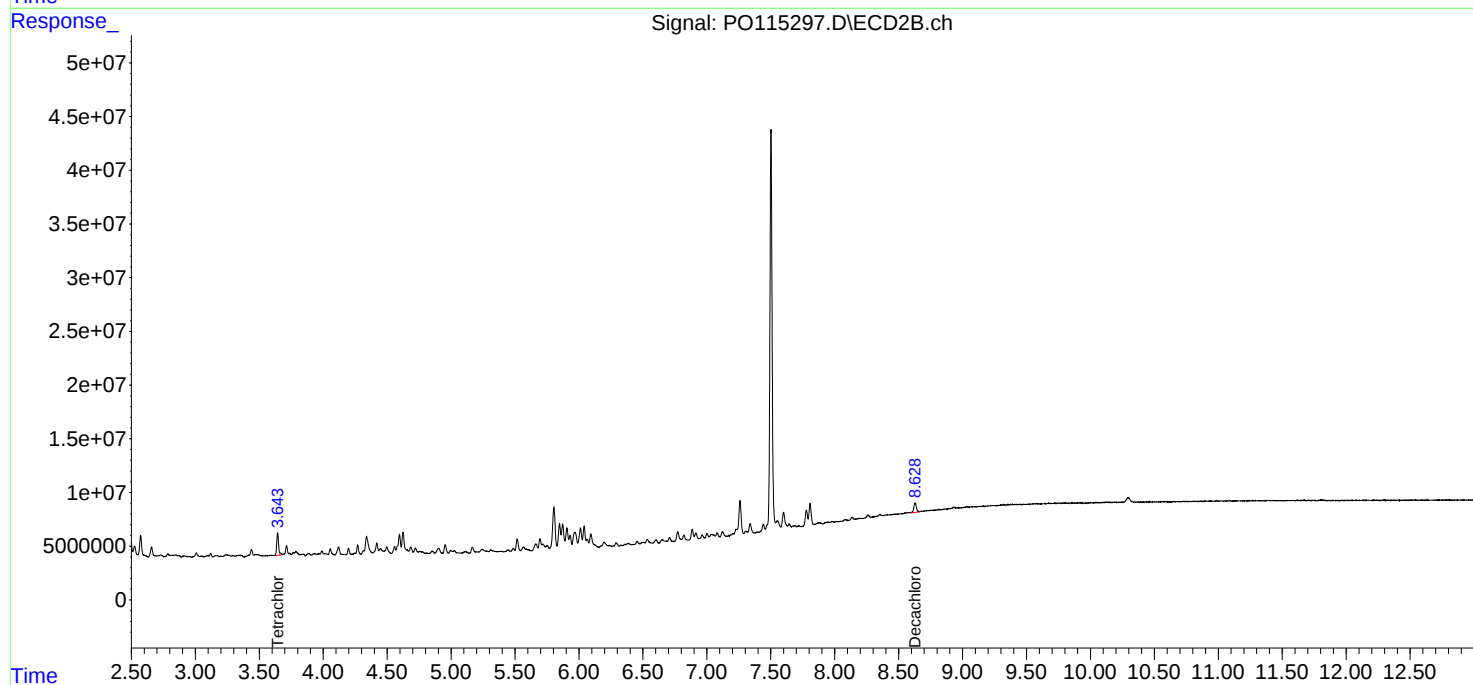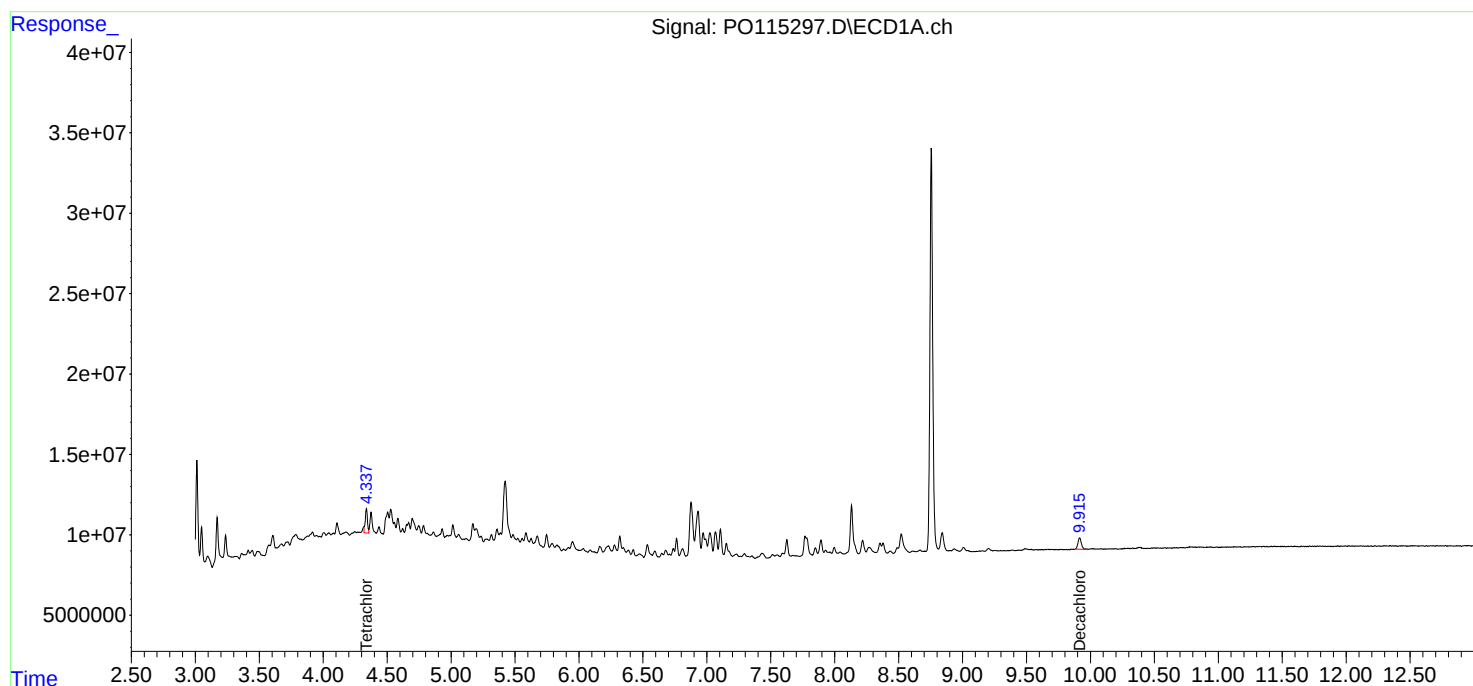

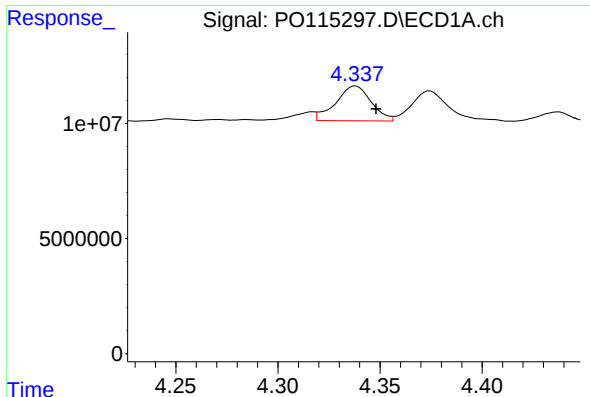


#1 Tetrachloro-m-xylene

R.T.: 4.337 min
Delta R.T.: -0.011 min
Response: 17892977
Conc: 2.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
BUR-25-0102


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/01/2025
Supervised By :Sohil Jodhani 12/01/2025

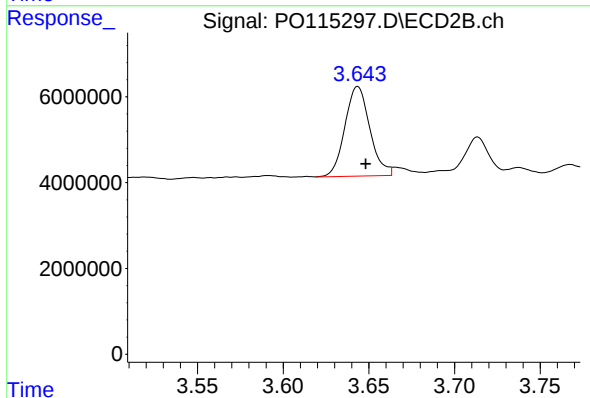


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.005 min
Response: 21198532
Conc: 4.75 ng/ml m

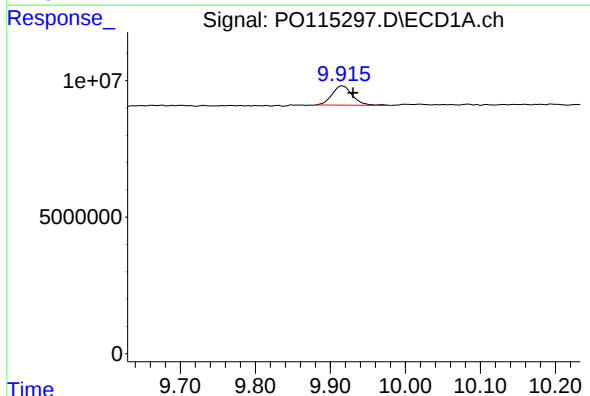

#2 Decachlorobiphenyl

R.T.: 9.916 min
Delta R.T.: -0.015 min
Response: 13348669
Conc: 3.02 ng/ml

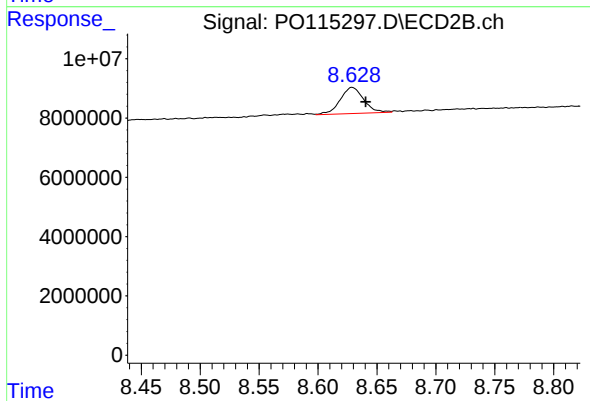

#2 Decachlorobiphenyl

R.T.: 8.629 min
Delta R.T.: -0.012 min
Response: 12265262
Conc: 3.14 ng/ml