

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112025\
 Data File : PO115300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2025 04:04
 Operator : YP/AJ
 Sample : Q3685-02 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 4198

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/21/2025
 Supervised By :Sohil Jodhani 12/01/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 05:38:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.338	3.643	10608207	12574658	1.507m	2.815 #
2) SA Decachlor...	9.921	8.634	5726733	5982397	1.296m	1.532

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112025\
Data File : PO115300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2025 04:04
Operator : YP/AJ
Sample : Q3685-02 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
4198


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/21/2025
Supervised By :Sohil Jodhani 12/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 05:38:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

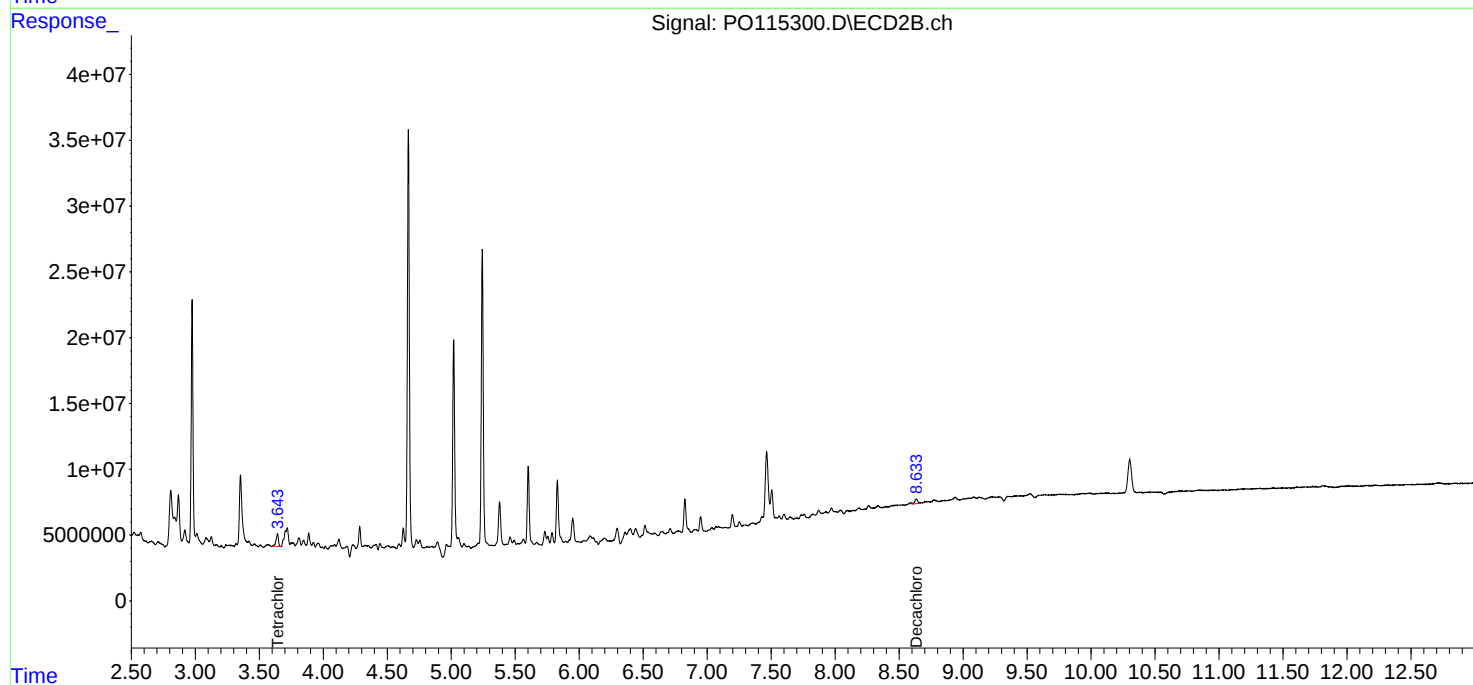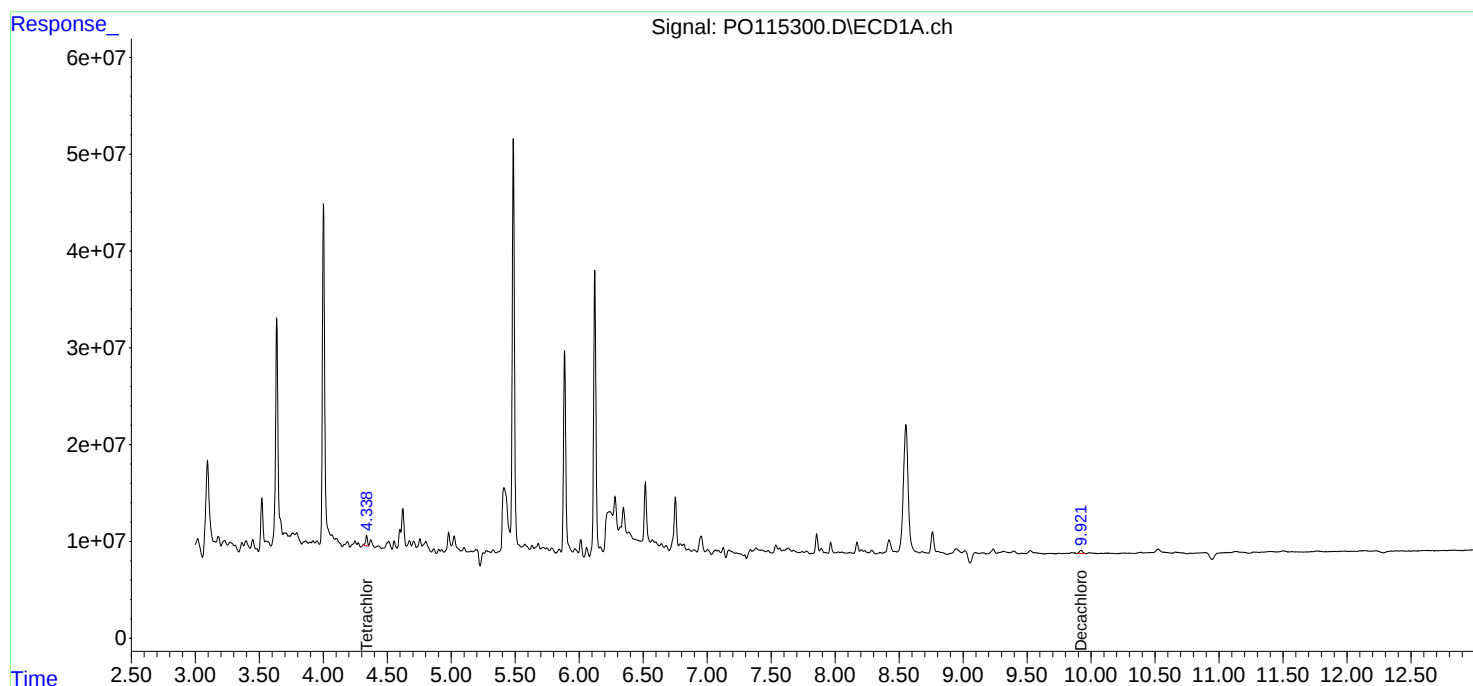

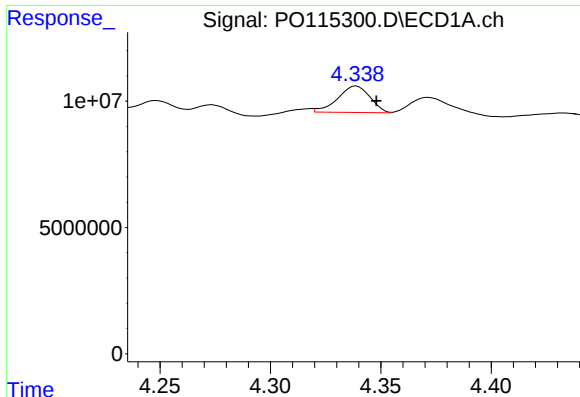


#1 Tetrachloro-m-xylene

R.T.: 4.338 min
Delta R.T.: -0.010 min
Response: 10608207
Conc: 1.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
4198


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/21/2025
Supervised By :Sohil Jodhani 12/01/2025

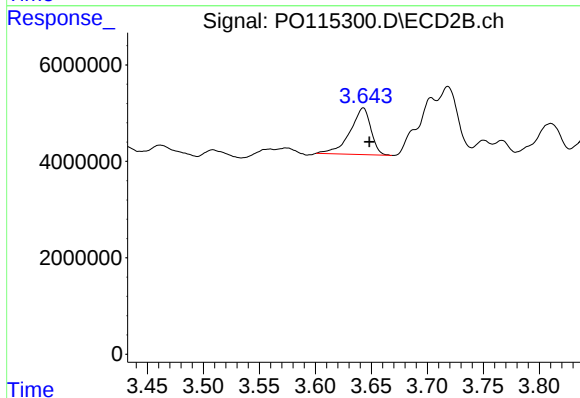


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.005 min
Response: 12574658
Conc: 2.82 ng/ml

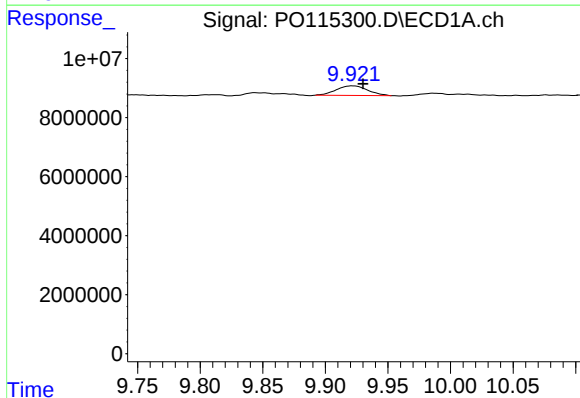

#2 Decachlorobiphenyl

R.T.: 9.921 min
Delta R.T.: -0.009 min
Response: 5726733
Conc: 1.30 ng/ml m

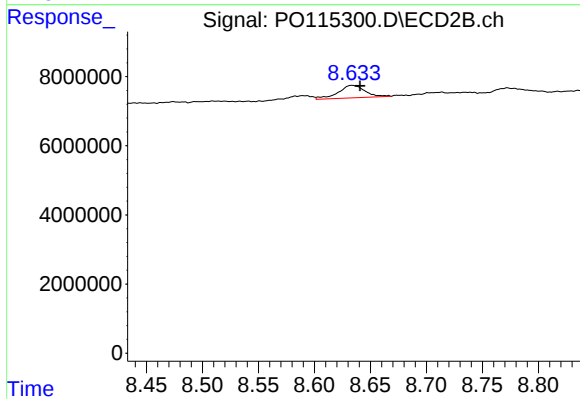

#2 Decachlorobiphenyl

R.T.: 8.634 min
Delta R.T.: -0.007 min
Response: 5982397
Conc: 1.53 ng/ml